

BEFORE THE HON’BLE NATIONAL GREEN TRIBUNAL
PRINCIPAL BENCH, NEW DELHI
OA NO. 1141 OF 2024

IN THE MATTER OF:-

Amresh Singh

....PETITIONER

VERSUS

State of UP & Ors.

....RESPONDENT

INDEX


S. No.	Particulars	Page No.
1.	Affidavit on behalf of the Respondent No. 5 - M/s Medical Pollution Control Committee in compliance of order dt. 20.11.2025 passed by this Hon’ble Tribunal	785-795
2.	Annexure R/1 - Copy of the CPCB Guidelines of December 2016	796 - 851
3.	Annexure R/2 – Copy of the Annual Report submitted under Form IV of the Environment Protection Rules, 1986, clarifying the abovementioned coverage of beds	852-855
4.	Annexure R/3 – Copy of the Letter dated 04.06.2025 by MPCC to Uttar Pradesh Pollution Control Board clarifying the reduction in the no. of beds due to new CBWTF facilities in the same distance.	856-857
5.	Annexure R/4 – Copy of the CPCB Guidelines for CBWTF dated April 2025.	858 - 922

6.	Annexure R/5 – Copy of the Methodology to Conduct gap analysis with respect to generation and treatment of biomedical waste” dated 10.10.2023.	923-925
7.	Proof of Service	926

Place: New Delhi

Date: 16.12.2025

FILED BY:



MANSI BACHANI, SURYA GUPTA and ANUBHAV ANAND

Enviro Legal Defence Firm,

29, Presidential Estate Nizamuddin East,

New Delhi -110013

eldflegal@gmail.com; 8600531203

SETTLED BY:

Sanjay Upadhyay

/Senior Advocate

BEFORE THE HON'BLE NATIONAL GREEN TRIBUNAL**PRINCIPAL BENCH, NEW DELHI****OA NO. 1141 OF 2024****IN THE MATTER OF:-**

Amresh Singh

....PETITIONER**VERSUS**

State of UP & Ors.

....RESPONDENT**AFFIDAVIT ON BEHALF OF THE RESPONDENT NO.5 - M/S MEDICAL****POLLUTION CONTROL COMMITTEE, IN COMPLIANCE OF THE****ORDER DT. 20.11.2025 PASSED BY THIS HON'BLE TRIBUNAL****MOST RESPECTFULLY SHEWETH:**

1. That the present case has been taken up by this Hon'ble Tribunal suo moto on 19.11.2024, in view of a complaint received by one Mr Amresh Singh, wherein it is has been alleged, albeit wrongly and without any basis in facts and law, that the Medical Pollution Control Committee (hereinafter referred as 'answering Respondent') has expanded its Common Bio Medical Waste Treatment Facility (CBMWTF) at Khalilabad, Sant Kabir Nagar without obtaining Environmental Clearance or consent.
2. That on 03.09.2025, this Hon'ble Tribunal had heard the final arguments and accordingly reserved its Judgment vide the said Order. Subsequently, this Hon'ble Tribunal, vide its order dated 18.11.2025, observed that some aspects of the case were not referred to at the time of the arguments and accordingly

directed the matter to be listed for the due elucidation/consideration on 20.11.2025.

3. That on 20.11.2025, this Hon'ble Tribunal directed the Answering Respondent herein to seek clarifications pertaining to the question of capacity of the CBWTF and the coverage area in compliance with CPCB Guidelines.
4. That in compliance of the Order dated 20.11.2025 of this Hon'ble Tribunal, the answering respondent is filing an affidavit clarifying the following –

I. Clarification regarding the coverage area of CBWTF

5. That at the outset, it is pertinent to mention that neither in the Letter Petition nor in any Additional Affidavit, the Original Applicant has raised the issue of coverage area vis a vis the Answering Respondent.
6. That specifically with respect to the clarification sought by this Hon'ble Tribunal, the CBWTF of the Answering Respondent at Sant Kabir Nagar, Khalilabad was granted the No-Objection Certificate for the establishment of its unit on 22.02.2008 [Annexed at Page 235 of the Reply dated 28.01.2025 by MPCC]. It is pertinent to mention that at the time of the establishment of the CBWTF unit, there were no provisions with respect to the coverage area for CBWTF either in the Bio-medical Waste Management Rules, 1998 or in the Guidelines specified by the Central Pollution Control Board.
7. That it was only after the enactment of the Bio-Medical Waste Management Rules, 2016, that the Central Pollution Control Board issued Guidelines in December 2016, prescribing the coverage area for CBWTF plants to be 75 km. The Guidelines further clarified that where 10,000 beds are not available in the coverage area of 75km, CBWTF may be allowed to extend the coverage area to 150km, provided that the waste is collected, treated and disposed of within 48 hours as stipulated in the BMW Rules. The true copy of the CPCB Guidelines of December 2016 is marked and annexed as **Annexure R/1**.

8. That the Authorisation for Bio-medical Waste was granted under the Bio-medical Waste Management Rules, 1998, on 24.04.2009 [Page 561 -563 of the Reply of MPCC dated 21.05.2025]. The latest Authorisation was granted on 18.09.2024, which is valid till 31.12.2028. The copy of the latest Authorisation is annexed at Page 280 of the Reply dated 28.01.2025 of MPCC. In compliance with the CPCB Guidelines of 2016, the coverage distance in Form III dated 18.05.2019 [Page 257 of the Reply dated 28.01.2025] for Authorisation under the Bio-Medical Waste Rules, 2016, clearly mentions that the coverage area of the CBWTF of the Answering Respondent includes –
 - a. Area/Distance is 150 km
 - b. No. of healthcare facilities is 888
9. That in compliance with the coverage distance in the Bio-Medical Authorisation, the Bio-Medical Waste Management Rules, 2016, and the CPCB Guidelines, the Answering Respondent's CBWTF was initially catering to 9897 beds [refer pg. 609 of the Reply of MPCC to the IA for Stay] within the 75km coverage radius. Thereafter, the number of healthcare facilities and beds was reduced to 1865 healthcare facilities [585 bedded hospital + 1280 non-bedded hospital] and 6202 beds in seven districts of Gorakhpur, Kushinagar, Santkabir Nagar, Siddharth Nagar , Maharajganj , Basti and Deoria due to registration of two new CBWTF facilities in the same coverage distance as the Answering Respondent. The Annual Report submitted under Form IV of the Environment Protection Rules, 1986, clarifying the abovementioned coverage of beds is marked and annexed herein at **Annexure R/2.**
10. That on 04.06.2025, the Answering Respondent has written to the Uttar Pradesh Pollution Control Board clarifying that due to the establishment of

two new CBWTF facilities, which are catering to Maharajganj, Kushinagar and Sindhant Nagar, eight Health Care Facilities with almost 4000 beds have moved from the Answering Respondent's facility to the two new CBWTF units. Hence, the Answering Respondent is now catering to about 5264 beds and should be allowed to register new health care facilities. The copy of the Letter dated 04.06.2025 is marked and annexed as **Annexure R/3**. Thus, at present, the unit of the Answering Respondent is working at a much reduced capacity. The details of the bed the CBWTF unit is catering to after the said letter is detailed below in furtherance of the instructions of the Answering Respondent –

District Name	Govt. HCF Beds	Private HCF Beds
Gorakhpur	1490	1838
Deoria	746	235
Maharajganj	0	325
Kushinagar	0	208
Sant KabirNagar	0	290
Sidharth Nagar	0	132
Total	2236	3028
Total beds (Govt. + Pvt)	5264 (2236+3028)	

11. That it is also pertinent to mention that the CPCB has issued the latest Guidelines on 12th April, 2025 for CBWTF units. The said Guidelines clarify the coverage area of 75km, however, the restriction on the number of beds is no longer there in the said Guidelines. For the purpose of determining the capacity, 90% of the total treatment capacity will be the criterion to determine the adequacy of the CBWTF in the coverage distance of 75km. The true copy

of the CPCB Guidelines of April 2025 is marked and annexed as **Annexure R/4**.

II. Clarification regarding the determination of Capacity

12. That the CBWTF unit of the Answering Respondent, in compliance of Para 9 of the Revised Guidelines for Common Bio-Medical Waste Treatment and Disposal Facilities dated 12.12.2016, has installed equipment such as Incinerator (double-chambered), Autoclave, Shredder and Effluent Treatment Plant with Zero Liquid Discharge (ZLD) on its premises for effective treatment of bio-medical waste.

13. That, as per the Authorization granted to the Answering respondent by UPPCB on 18.09.2024, capacity of the following equipment are –

S. NO.	EQUIPMENT	CAPACITY
1.	Incinerator (double-chambered)	100 Kg/Hour
2.	Autoclave	500 Ltr./Batch
3.	Shredder	50 Kg/Hour
4.	Effluent Treatment Plant with Zero Liquid Discharge (ZLD)	10.0 KLD

14. That further, while considering the abovementioned newly installed equipment, the total capacity of the CBWTF is calculated as below –

- 100 Kg Incinerator (20 hours per day) = 2000 Kg/Day
- 500 Litre/hours (8 hours per day) + 50 Kg Shredder & Chemical Disinfection = 4500 Kg/Day
- Hence, total capacity = 6500 Kg/Day

Capacity of Medical Pollution Control Committee CBWTF
D – 33, UPSIDC Industrial Area, Khalilabad, Santkabirnagar – 272175

- 100 Kg Incinerator X 20 Hours = 2000 Kg
 - 500 liter /hours X 8 Hours
 - 50 Kg Shredder & Chemical Disinfection
- } = 4500 Kg/Day
- Total Capacity = 6500 Kg/Day**

15. That as per the abovementioned calculations and the Answering Respondent's Annual report dated 24.06.2025, the installed capacity of the CBWTF for the treatment of bio-medical waste is 6,500 Kg per day. Though, the actual quantity of bio-medical waste currently treated and disposed of by the same amounts to 1,095 Kg per day as per the last Annual Report of 24.06.2025.

16. That as per the "Methodology to Conduct gap analysis with respect to generation and treatment of biomedical waste" dated 10.10.2023 issued by CPCB, the time period taken for calculating the existing capacity from incinerator is laid down as 20 hrs/day and for autoclave, it is 18 cycles per day. Further, the average time period for completion of one cycle for autoclave takes approximately one hour to complete, which translates the capacity for autoclave to eighteen hours/day. That as per these figures, the total capacity comes out to be much more than the capacity sanctioned of 6500 kg/day for the CBMWTF of the answering Respondent.

That the true copy of the "Methodology to Conduct gap analysis with respect to generation and treatment of biomedical waste" dated 10.10.2023 is marked and annexed as **Annexure R/5**.

17. That 274 grams of biomedical waste is generated per day per bed. Out of total Bio-Medical Waste collected, approximately 20 to 25% is transferred to

incinerable waste and remaining 75 to 80% of the waste is treated using autoclaving or shredded and chemical disinfectants to ensure it is sterilized and rendered safe for disposal in accordance with the Bio-Medical Waste Rules, 2016. However, at present, due to 4000 beds being catered by another CBWTF facility, the Answering Respondent's CBWTF facility is completely underutilised.

18. It is humbly submitted that even under the New Guidelines of April 2025 and owing to the fact that the R-5 is now catering to only about 5264 beds, the compliance with the new guidelines is also adequate and in fact could be increased subject to demand. Thus, for example, as per the new guidelines, the per-bed calculations of biomedical waste generated, if it is assumed that all 5264 are bedded HCF facilities, is about -

$$5264 * 0.277 \text{ kg/day} = 1458.128 \text{ kg/day} .$$

Hence, even as per the calculations of the April, 2025 Guidelines, the Answering Respondent will be compliant with its coverage and capacity. Further, as per the April, 2025 Guidelines, 90% of the capacity of the unit of the Answering Respondent is to be considered for assessing whether there is a requirement of a new CBWTF. The approved capacity of the CBWTF unit of the Answering Respondent is 6500kg/day. Thus, if the unit of the Answering Respondent works at 100% capacity, the total no. of beds would be –

$$6500/0.277 = 23465 \text{ beds (approximately)}$$

Accordingly, 90% of 23465 beds come to 21,119 beds (approximately). Thus, the unit of the Answering Respondent is working with 5264 beds at present, which is clearly much lower than the 90% approved capacity.


19. That in view of the abovementioned facts, it is submitted that Answering Respondent has undertaken its operations and activities in accordance with

law and the present case filed by the Letter Applicant is frivolous and is liable to be dismissed with huge cost.

Place: New Delhi

Date: 16.12.2025

FILED BY:

A handwritten signature in blue ink, reading 'Mbachani', with a horizontal line underneath.

MANSI BACHANI, SURYA GUPTA & ANUBHAV ANAND

Enviro Legal Defence Firm,

29, Presidential Estate Nizamuddin East,

New Delhi -110013

eldflegal@gmail.com; 8600531203

SETTLED BY:

Sanjay Upadhyay

[Senior Advocate]

THE HON'BLE NATIONAL GREEN TRIBUNAL
PRINCIPAL BENCH, AT NEW DELHI
ORIGINAL APPLICATION NO. 1141 OF 2024

IN THE MATTER OF:

Amresh Singh

... Applicant

-Versus-

State of Uttar Pradesh & Ors.

... Respondents

AFFIDAVIT

I, Dr. Vinay Kumar Verma, aged about 65 years, S/o Late Rajaram Verma R/o 26A-B, Block E, near Bhatia Hotel, Panki, Kanpur, Uttar Pradesh – 208020, Secretary and authorized signatory of Medical Pollution Control Committee (MPCC), do hereby solemnly affirms and declares as under:

1. That in my capacity as Respondent No. 5 in the abovementioned matter I am fully conversant with the facts and circumstances of the case, as such I am competent to swear to this affidavit.
2. The contents of the accompanying Reply have been drafted by the counsel under my instructions and the contents of the same are true and correct to my knowledge and no part of it is false and nothing material has been concealed therefrom.
3. Annexures are the true copy of their respective original.

Dr. Vinay Kumar Verma
DEPONENT

VERIFICATION:

Verified at _____ on this _____ day of December, 2025
that the contents of the above affidavit are true and correct to my knowledge and belief and nothing material has been concealed there from.

Notified that this documents
presented before me for
verification
is identified by me
and is true and correct
as per the information
provided

Dr. Vinay Kumar Verma
DEPONENT

SUJEET KUMAR ADVOCATE
Government Notary
Govt. of India

Revised Guidelines for Common Bio-medical Waste Treatment and Disposal Facilities



CENTRAL POLLUTION CONTROL BOARD

(Ministry of Environment, Forest and Climate Change)

Parivesh Bhawan, East Arjun Nagar

DELHI -110 032

website: www.cpcb.nic.in

(December 21, 2016)

Abbreviations

APCD	-	Air Pollution Control Device
BMWM Rules	-	Bio-medical Waste Management Rules
CBWTF	-	Common Bio-medical Waste Treatment and Disposal Facility
CO	-	Carbon Monoxide
CO ₂	-	Carbon Dioxide
CPCB	-	Central Pollution Control Board
CRZ	-	Coastal Regulation Zone
DG	-	Diesel Generator
EC	-	Environmental Clearance
EIA	-	Environment Impact Assessment
ETP	-	Effluent Treatment Plant
GPS	-	Global Positioning System
HCFs	-	Health Care Facilities
HCl	-	Hydrochloric Acid
HOWM & TM Rules	-	Hazardous and Other Waste (Management & Transboundary Movement) Rules, 2016
MHz	-	Mega Hertz
MoEF& CC	-	Ministry of Environment, Forest & Climate Change
KM	-	Kilometer
KW	-	Kilowatt
MoU	-	Memorandum of Understanding
NABL	-	National Accreditation Board for Testing and Laboratories
NO _x	-	Oxides of Nitrogen
O ₂	-	Oxygen
PCC	-	Pollution Control Committee
PLC	-	Programmable Logical Control
SEIAA	-	State Environment Impact Assessment Authority
SLF	-	Secured Landfill
SPCB	-	State Pollution Control Board
TSDF	-	Treatment Storage and Disposal Facility
TOC	-	Total Organic Carbon
VOCs	-	Volatile Organic Compounds

CONTENT

S. No	Description	Page No.
1	Introduction	01
2	Criteria for development of a new Common Bio-medical Waste Treatment and Disposal Facility	02
3	Duties of the operator of a common bio-medical waste treatment and disposal facility	06
4	Applicability of the guidelines	06
5	Environmental laws applicable for commissioning or operation of a CBWTF	07
6	Location criteria	08
7	Land requirement	09
8	Coverage area of CBWTF	10
9	Treatment equipment	10
10	Infrastructure set up	15
11	Record keeping	20
12	Collection and transportation of bio-medical waste	25
13	Disposal option of solid waste generated from CBWTF	27
14	Cost to be charged by the CBWTF operator for the Health Care Facilities	29
15	Check list for development of CBWTF	29
16	Periodic inspection/monitoring or performance evaluation of the CBWTFs	30
	List of Figure and Table	
	Figure 1. Criteria for development of a CBWTF in a coverage area	05
	Table 1: Suggested validation test for treatment of bio-medical waste by autoclave/microwave/chemical treatment/dry heat sterilization	24
	Table 2: Suggested disposal option of solid waste generated from CBWTF	28
	List of Annexure	
	Annexure-I: Coverage area-wise gap analysis for assessing additional BMW treatment capacity requirement	31
	Annexure -II: Format for maintaining the record by the CBWTF Operator along with the transportation vehicle used for collection of the Bio-medical waste from the member HCFs	32
	Annexure -III: Log Book for operating the Incinerator/Plasma Pyrolysis and Autoclave	33
	Annexure -IV: Check list for Development of a CBWTF	34
	Annexure -V: Check list for Performance Evaluation of the CBWTF	38
	Annexure -VI: Stationary Source Emission Monitoring for Dioxins and Furans	50
	References	53

1) Introduction

A Common Bio-medical Waste Treatment and Disposal Facility (CBWTF) is a set up where biomedical waste generated from member health care facilities is imparted necessary *treatment* to reduce adverse effects that this waste may pose on human health and environment. The treated recyclable waste may finally be sent for disposal in a secured landfill or for recycling.

According to the Bio-medical Waste Management Rules, 2016, "*bio-medical waste treatment and disposal facility*" means any facility wherein treatment, disposal of bio-medical waste or processes incidental to such treatment and disposal is carried out, and includes common bio-medical waste treatment facilities and "*operator of a common bio-medical waste treatment facility*" means a person who owns or controls a Common Bio-medical Waste Treatment and Disposal Facility (CBWTF) for the collection, reception, storage, transport, treatment, disposal or any other form of handling of bio-medical waste.

The Bio-medical Waste Management Rules, 2016 (hereafter referred as BMW Rules) restricts occupier for establishment of on-site or captive bio-medical waste treatment and disposal facility, if a service of common bio- medical waste treatment and disposal facility is available within a distance of seventy-five kilometer, as installation of individual treatment facility by health care facility (HCF) requires comparatively high capital investment. In addition, it requires separate dedicated and trained skilled manpower and infrastructure development for proper operation and maintenance of treatment systems. The concept of *CBWTF* is not only addresses such problems but also prevents proliferation of treatment technologies in a particular town or city. In turn, it reduces the monitoring pressure on regulatory agencies. By running the treatment equipment at CBWTF to its full capacity, the cost of treatment of per kilogram bio-medical waste gets significantly reduced. Its considerable advantages have made CBWTF popular and proven concept in most part of the world.

The CBWTFs are also required to set up based on the need for ensuring environmentally sound management of bio-medical waste keeping in view the techno-economic feasibility and viable operation of the facility with minimal impact on human health and environment.

Since 1998, the CBWTF as an option for treatment of bio-medical waste also been legally introduced in India. Considering the likely impacts that may cause to the patients undergoing treatment because of operation of the captive treatment

equipment within the health care facilities (HCFs), now the Bio-medical Waste Management Rules, 2016 restricts the Occupier (i.e., HCF) for ensuring treatment and disposal of generated bio-medical waste through a CBWTF, located within a distance of 75 KM. Further, these rules eased the bottleneck in upbringing the CBWTF by making department in the business allocation of land assignment in the State or UT administration responsible for providing a suitable site (s) within its jurisdiction.

The concept of CBWTF is also being widely accepted in India among the healthcare units, medical associations and entrepreneurs. In order to set up a CBWTF to its maximum perfection, care shall be taken in choosing the right technology, development of CBWTF area, proper designing of transportation system to achieve optimum results etc. Key features of CBWTF have been addressed in the subsequent sections.

To facilitate the treatment and disposal of bio-medical waste generated from the HCFs, at present (as per Annual Report 2014 submitted by the SPCBs/PCCs), there are 192 no. of CBWTFs in operation and 33 no. of CBWTFs are under construction. Also, the Bio-medical Waste Management Rules, 2016 mandates that the operator of a CBWTF authorised by the prescribed authority is required to take all necessary steps to ensure that the bio-medical waste collected from the occupier is transported, handled, stored, treated and disposed of, without any adverse effect to the human health and the environment, in accordance with the BMW Rules and the guidelines issued by the Central Government or the Central Pollution Control Board (CPCB) from time to time. Therefore, these guidelines have been prepared with an aim to have uniformity in ensuring site selection, allowing and establishment of a state-of-the-art CBWTF, operation as well as verification of compliance to the BMW Rules, 2016 throughout the country. However, any other aspects which are not been covered under these guidelines and needs attention, in such a case, the prescribed authority may take suitable action in the interest of protection of the environment in consultation with MoEF & CC/CPCB. Also, it is pertinent to mention here that these guidelines are mandatory henceforth under the Bio-medical Waste Management Rules, 2016

2) Criteria for development of a new Common Bio-medical Waste Treatment and Disposal Facility for a locality or region.

Prior to allowing any new CBWTF, following criteria or steps may be followed:

- a) Prescribed authority under the BMW Rules, 2016 [i.e., State Pollution Control Board (SPCB) in the respective State or Pollution Control Committee (PCC) in the respective

Union Territory Administration] is required to prepare an inventory or review with regard to the bio-medical waste generation at least once in five years in the coverage areas of the existing bio-medical waste treatment and disposal facility. The prescribed authority is also required to extrapolate the coverage-area wise bio-medical waste generation for the next ten years.

- b) SPCB/PCC is required to conduct gap analysis w.r.to coverage area of the bio-medical waste generation and also projected over a period of next ten years, adequacy of existing treatment capacity of the CBWTF in each coverage area of radius 75 KM, as given in **Annexure-I**.

All the SPCBs and PCCs shall conduct the gap analysis and based on the gap analysis, action plan for development of new CBWTFs is required to be prepared and submitted to MoEF & CC & CPCB within six months' time. In case of States/UTs, where no CBWTF is available, in such a case, SPCB/PCC being prescribed authority under the BMW Rules is required to submit the detailed proposal to MoEF & CC/MoH & FW through the respective State Government or UT Administration. Also, the option of forming association by the group of health care facilities (HCFs) to develop their own CBWTF also be encouraged following these guideline. In case, any coverage area requires additional treatment capacity, in such a case, action may be initiated by the prescribed authority for allowing a new CBWTF in that locality without interfering the coverage area of the existing CBWTF and beds covered by the existing CBWTF.

- c) SPCB/PCC shall identify the coverage area, which require additional treatment facility and bring it to the notice of the concerned department in the business allocation of land assignment in the respective State Government or UT Administration. The department in the business allocation of land assignment shall be responsible for providing suitable site in the identified coverage area for setting up of a CBWTF, in consultation with the prescribed authority (i.e., SPCB/PCC), other stakeholders and in accordance with these guidelines issued by CPCB from time to time.
- d) Alternately, a CBWTF may also be allowed to be established on a land procured by an entrepreneur in accordance with the location criteria suggested under these guidelines.
- e) The SPCB/PCC or concerned department in the business allocation of land assignment in the respective State Government or UT Administration may seek expression of interest from the proponents for development of new CBWTF (s) in the identified coverage area. Upon allocation of site to the proponent, the proponent is
-

required to take necessary approvals as required under the Environment (Protection) Act, 1986 for development of the new CBWTF in accordance with these guidelines.

- f) In the absence of expression of interest by any proponent, then SPCB/PCC shall insist health care facilities to form association and to develop its own CBWTF in line with these guidelines or to have captive treatment facilities for ensuring treatment and disposal of generated bio-medical waste as stipulated under the BMWWM Rules, 2016.
- g) In case of any regulatory action including closure of any existing CBWTF is inevitable, the respective SPCB/PCC may take action under the BMWWM Rules including for making alternate arrangement to ensure safe disposal of the bio-medical waste generated from the member health care facilities of such default CBWTF through CBWTF located nearby.
- h) In case of hilly areas considering the geography, only one CBWTF with adequate treatment capacity may be developed covering atleast two districts to cater treatment services to the HCFs located in the respective Districts. The selection and allocation of site etc., should be done as per the criteria suggested under these guidelines. The treatment charges to be prescribed by the respective SPCB/PCC in consultation with the State Advisory Committee.

The criteria for development of CBWTFs in any coverage area is also depicted in **Figure 1**.



3) **Duties of the operator of a common bio-medical waste treatment and disposal facility**

The duties of the operator of a common bio-medical waste treatment and disposal facility (CBWTF) as enunciated under Rule 5 of the Bio-medical Waste Management Rules, 2016 shall be ensured and complied with. Also, all the existing CBWTFs shall also complete augmentation of the existing incineration facility so as to comply w.r.to the residence time as well as emission norms including for Dioxins and Furans prescribed under BMWM Rules, 2016 within two years from the date of notification of the BMWM Rules, 2016 (i.e., prior to 27.03.2018). In addition to the above, to ensure proper management of bio-medical waste in the respective coverage area, as a mitigation measure, especially in the event of

- (a) a temporary break down (not more than a week) of a CBWTF especially for rectification of the refractory lining of the incineration chambers or change of requisite APCD due to failure; and
- (b) Closure of a CBWTF for violation of the provisions of the BMWM Rules or any other reason.

Prior to commencement of a new CBWTF as well as all the existing CBWTF Operators are required to submit action plan, to the respective SPCB/PCC, for imposing suitable condition while granting authorisation under the BMWM Rules, 2016. The action plan should also include:

- (a) a MoU made with the nearest CBWTF located within the respective State/UT, as alternate arrangement. In case, if there is no CBWTF located nearby then such CBWTF should have to install stand by treatment equipment (equal to the existing treatment capacity as per consents granted by the SPCB/PCC), and
- (b) decontamination plan of the CBWTF for execution of such plan prior to closure of a CBWTF.

4) **Applicability of these guidelines**

These guidelines are applicable to all the upcoming or new CBWTFs. In case of the existing CBWTFs, these guidelines shall be applicable in case

- (a) the existing CBWTFs desires to expand or enhance the existing treatment capacity
(or)
- (b) the existing CBWTFs desires to modernize the existing treatment equipment with the new equipment with enhancement in the existing treatment capacity.

5) **Environmental laws applicable for commissioning or operation of a CBWTF**

Operation of a CBWTF leads to air emissions as well as waste water generation as in case of an industrial operation. Most common sources of waste water generation in CBWTFs are vehicle washing, floor washing, and scrubbed liquid effluent from air pollution control systems attached with the incinerator/plasma pyrolysis. Incineration as well as DG Set is the general source of air emissions.

5.1 Any other approvals (such as Land Use /Change in Land Use as applicable) required from the concerned authorities under various laws have to be complied with by the proponent of the CBWTF prior to development of a CBWTF.

5.2 Consents under Water (Prevention and Control of Pollution) Act, 1974 and Air (Prevention and Control of Pollution) Act, 1981 as well as Authorization under the BMW Rules, 2016

The project proponent of the CBWTF is required to obtain 'Consent to Establishment' under Rule 25 of the Water (Prevention and Control of Pollution) Act, 1974 and under Rule 21 of the Air (Prevention and Control of Pollution) Act, 1981, from the respective prescribed authority i.e. SPCB/PCC. Upon installation of the requisite equipment, the CBWTF Operator is also required to obtain authorization under BMW Rules, 2016 co-terminus with consent to operate under Water (Prevention and Control of Pollution) Act, 1976 & Air (Prevention and Control of Pollution) Act, 1981 from the respective SPCB/PCC prior to commencement of the CBWTF.

5.3 Environmental Clearance under EIA Notification 2006

Ministry of Environment, Forest & Climate Change (MoEF & CC), notified amendment to the EIA Notification 2006 and published vide MoEF & CC Notification of S.O. 1142 (E) dated April 17, 2015. According to this notification, the 'bio-medical waste treatment facility' is categorized under the Item 7 (da) in the schedule, requiring 'environmental clearance' from the State Environment Impact Assessment Authority (SEIAA). Therefore, the CBWTF operator is also required to obtain 'Environmental Clearance (EC)' from the respective SEIAA or Ministry of Environment, Forest & Climate Change (MoEF & CC), as the case may be, before any construction work, or preparation of land by the projects management, which include the following:

- a) All new projects or activities pertaining to the bio-medical waste treatment facility; and
- b) Expansion and modernization with additional treatment capacity of existing bio-medical waste treatment facility (excluding augmentation of incineration facility)

for compliance to the residence time as well as Dioxins and Furans without enhancing the existing treatment capacity).

- c) Any expansion or modification in the treatment capacity or relocation of the existing CBWTF (requires compliance to the relevant provisions notified under the Environment (Protection) Act, 1986 by the MoEF & CC

6) Location criteria

In the context of these guidelines, buffer zone represents a separation distance between the source of pollution in CBWTF and the receptor - following the principle that the degree of impact reduces with increased distance. The following parameters may be considered for ascertaining buffer distance on case-to-case basis:

- (i) potential for spread of infection from wastes stored in the premises.
- (ii) applicable standards for pollution control and the relative efficiency of the existing incinerators and emission control systems,
- (iii) potential of fugitive dust emission from incinerators,
- (iv) potential for discharge of wastewater
- (v) the potential for odour production,
- (vi) the potential for noise pollution,
- (vii) the risk posed to human health and safety due to exposure to emissions from incinerator,
- (viii) the risk of fire and
- (ix) Significance of the residual impacts such as bottom ash and fly ash.

As far as possible, the CBWTF shall be located near to its area of operation in order to minimize the transportation distance in waste collection, thus enhancing its operational flexibility as well as for ensuring compliance to the time limit for treatment and disposal of bio-medical waste as stipulated under the BMWM Rules (i.e., within 48 hours). Also, the location of the CBWTF should be in conformity to the CRZ Norms and other provisions notified under the Environment (Protection) Act, 1986. The location shall be decided in consultation with the State Pollution Control Board (SPCB)/ Pollution Control Committee (PCC). The location criteria for development of a CBWTF are as follows:

- (a) A CBWTF shall preferably be developed in a notified industrial area without any requirement of buffer zone **(or)**
- (b) A CBWTF can be located at a place reasonably far away from notified residential and sensitive areas and should have a buffer distance of preferably 500 m so that it shall

have minimal impact on these areas. In case of non-availability of such a land, the buffer zone distance from the notified residential area may be reduced to less than 500 m by SPCB/PCC without referring the matter to CPCB by prescribing additional control measures such as (i) adoption of best available technologies (BAT) by the proponent of CBWTF; (ii) prescribing stringent standards for operation of the CBWTF by the SPCB/PCC; (iii) adoption of zero liquid discharge by the CBWTF and (iv) in case of any complaints from the public, then CBWTF should prove that the facility is not causing any adverse impact on environment and habitation in the vicinity. If SPCB/PCC is not in a position to resolve the issue relating to buffer zone while selecting the site for CBWTFs, in such a case, SPCBs/PCCs may refer the matter to CPCB.

- (c) The CBWTF can also be developed as an integral part of the Hazardous Waste Treatment Storage and Disposal Facility (TSDF) subject to obtaining of necessary approvals from the authorities concerned including 'environmental clearance' as per Environmental Impact Assessment 2006 and further amendments notified under the Environment (Protection) Act, 1986, provided there is no CBWTF exist within 150 KM distance from the existing TSDF.

7) Land requirement

Sufficient land shall be allocated to the CBWTF to provide all requisite systems which include dedicated space for storage of waste (both treated and untreated), waste treatment equipment, vehicle washing bay, vehicle parking space, ETP, incineration ash storage provision, administrative room, space for DG Set etc.,.

- (a) Preferably, a CBWTF shall be set up on a plot size of not less than one acre in all the areas. However, a CBWTF can be developed in adjacent plots but cannot be set up in two or more different plots located in different areas. Separate plots can be permitted only for vehicle parking if located in the close vicinity of the proposed CBWTFs or the existing CBWTFs.
- (b) In case of upcoming or new CBWTFs (both in municipal limits with population more than 25 lakhs or in rural areas), the land area requirement may be relaxed (but in any case not less than 0.5 acre) by the SPCB/PCC, with additional control measures such as zero liquid discharge, increase in stack height, stringent emission norms, odour control measures or any other measures felt necessary by the prescribed authority on case-to-case basis, only in consultation with CPCB.

8) Coverage area of CBWTF

Suggested coverage area for development of a CBWTF is as follows:

- a) A CBWTF located within the respective State/UT shall be allowed to cater healthcare units situated at a radial distance of 75 KM. However, in a coverage area where 10,000 beds are not available within a radial distance of 75 KM, existing CBWTF in the locality (located within the respective State/UT) may be allowed to cater the healthcare units situated upto 150 KM radius w.r.to its location provided the bio-medical waste generated is collected, treated and disposed of within 48 hours as stipulated under the BMWM Rules.
- b) In case, number of beds is exceeding >10,000 beds in a locality (i.e. coverage area of the CBWTF under reference) and the existing treatment capacity is not adequate, in such a case, a new CBWTF may be allowed in such a locality in compliance to various provisions notified under the Environment (Protection) Act, 1986, to cater services only to such additional bed strength of the HCFs located.
- c) In case of hilly areas, considering the geography, only one CBWTF with adequate treatment capacity may be developed covering atleast two districts to cater treatment services to the HCFs located in the respective Districts. The selection and allocation of site etc. should be done as per the criteria suggested under these guidelines. The treatment charges to be prescribed by the respective SPCB/PCC in consultation with the State Advisory Committee to be constituted under the BMWM Rules by the respective State Government or UT Administration.

9) Treatment equipment

The Common Bio-medical Waste Treatment Facility should treat the bio-medical waste as per BMWM Rules and as per the authorisation granted by the prescribed authority. The CBWTF should have the following treatment facilities:

a) *Incineration/Plasma Pyrolysis*

Incineration is a controlled combustion process where waste is completely oxidized and harmful microorganisms present in it are destroyed/ denatured under high temperature. The guidelines for "Design & Construction Requirements of Bio-medical Waste Incinerators" by CPCB from time to time shall be followed for selecting/or augmenting the incinerator.

Plasma Pyrolysis is an alternate to incinerator, Plasma Pyrolysis treatment technology can be installed for disposal of bio-medical waste categories as per BMWM Rules wherein destruction of bio-medical waste is similar to incineration can be achieved. In case of plasma pyrolysis, waste is treated at high temperature under controlled condition to form gases like methane, hydrogen and carbon monoxide which are subjected to combustion (oxidation) in secondary chamber. In the plasma pyrolysis process waste is converted into small clinker which can be disposed in secured landfills.

b) Autoclaving/Hydroclaving

- (i) Autoclaving** is a low-heat thermal process where steam is brought into direct contact with waste in a controlled manner and for sufficient duration to disinfect the wastes as stipulated under the Bio-medical Waste Management Rules. For ease and safety in operation, the system should be horizontal type and exclusively designed for treatment of bio-medical waste. For optimum results, pre-vacuum based system be preferred against the gravity type system. It shall have tamper-proof control panel with efficient display and recording devices for recording critical parameters such as time, temperature, pressure, date and batch number etc. as required under the BMWM Rules.
 - (ii) Hydroclaving** is similar to that of autoclaving except that the waste is subjected to indirect heating by applying steam in the outer jacket. The waste is continuously tumbled in the chamber during the process.
 - c) Microwaving:** In microwaving, microbial inactivation occurs as a result of the thermal effect of electromagnetic radiation spectrum lying between the frequencies 300 and 300,000MHz. Microwave heating is an inter-molecular heating process. The heating occurs inside the waste material in the presence of steam.
 - d) Chemical disinfection:** Though chemical disinfection or alternates as stipulated under the BMWM Rules is also an option for treatment of certain categories of bio-medical waste such as glass waste but looking at the volume of waste to be disinfected at the CBWTF and the pollution load associated with the use of chemical disinfectants, the chemical disinfection for treatment of bio-medical waste as part of a CBWTF may be used sparingly or avoided as far as possible.
 - e) Dry heat sterilization:** This is the additional option for treatment of waste sharps as stipulated under the BMWM Rules. In this method, waste sharps are treated using
-

dry heat (hot air) at a temperature not less than 185°C, at least for a residence period of 150 minutes in each cycle (with sterilization period of 90 minutes).

f) *Shredder:* Shredding is a process by which waste are de-shaped or cut into smaller pieces so as to make the wastes unrecognizable. It helps in prevention of reuse of bio-medical waste and also acts as identifier that the wastes have been disinfected and are safe to dispose off. A shredder to be used for shredding bio-medical waste shall confirm to the following minimum requirements:

- (i) The shredder for bio-medical waste shall be of robust design with minimum maintenance requirement;
- (ii) The shredder should be properly designed and covered to avoid spillage and dust generation. It should be designed such that it has minimum manual handling;
- (iii) The hopper and cutting chamber of the shredder should be so designed to accommodate the waste bag full of bio-medical waste;
- (iv) The shredder blade should be highly resistant and should be able to shred waste sharps, syringes, scalpels, blades, plastics, catheters, intravenous sets/ bottles, blood bags, gloves, bandages etc. It should be able to handle/ shred wet waste, especially after microwave/ autoclave/hydroclave;
- (v) The shredder blade shall be of non-corrosive and hardened steel;
- (vi) The shredder should be so designed and mounted so as not to generate dust, high noise & vibration;
- (vii) If hopper lid or door of collection box is opened, the shredder should stop automatically for safety of operator;
- (viii) In case of shock-loading (non-shreddable material in the hopper), there should be a mechanism to automatically stop the shredder to avoid any emergency/accident;
- (ix) In case of overload or jamming, the shredder should have mechanism of reverse motion of shaft to avoid any emergency/accident;
- (x) The motor shall be connected to the shredder shaft through a gear mechanism, to ensure low rpm and safety;
- (xi) The unit shall be suitably designed for operator safety, mechanical as well as electrical;
- (xii) The shredder should have low rotational speed (maximum 50 rpm). This will ensure better gripping and cutting of the bio-medical waste;

- (xiii) The discharge height (from discharge point to ground level) shall be sufficient (minimum 3 feet) to accommodate the containers for collection of shredded material. This would avoid spillage of shredded material;
- (xiv) The minimum capacity of the motor attached with the shredder shall be 3 KW for 50 Kg/hr, 5 KW for 100 kg/hr & 7.5 KW for 200 Kg/hr and shall be three phase induction motor. This will ensure efficient cutting of the bio-medical wastes as prescribed in the Bio-medical Waste Management Rules; and
- (xv) The shredder also should be fitted with separate 'energy meter' for recording total energy consumed for operation of this equipment.

g) *Sharp pit/ Encapsulation:* A sharp pit or a facility for sharp encapsulation in a metal container or cement concrete shall be provided for treated sharps (*i.e., treatment by autoclaving or dry heat sterilization followed by shredding or mutilation*). An option may also be worked out for recovery of metal from treated and shredded waste sharps within the CBWTF or iron foundries having consent to operate from the SPCBs/PCCs and located nearby, as per the conditions imposed in authorization granted under BMWM Rules by the SPCB/PCC.

A sharp pit may be of circular or rectangular shape and shall be dug and lined with cement plastered brick masonry or concrete rings. The pit should be covered with a heavy concrete slab with a provision of galvanized steel pipe projecting about 1.5 meters above the slab, with an internal diameter of up to 50 mm or 1.5 times the length of vials, whichever is more. The top opening of the steel pipe shall have a provision of locking after the treated waste sharps are disposed into the sharp pit. When the pit is full, it can be sealed completely, after another pit is prepared. In case of high water table regions (*i.e., where water table is less than 6 metres beneath the bottom of the sharp pit*), a tank with above mentioned arrangements shall be made above the ground.

h) *Deep burial:* Any SPCB/PCC should not allow the 'deep burial' of bio-medical waste as a part of CBWTF. Any existing CBWTF having disposal of bio-medical waste by deep burial should have the requisite treatment equipment as stipulated under the BMWM Rules, *within six months* from the date of finalization of these guidelines.

i) *Non-burn technology:* Non-incineration technologies for disposal of bio-medical waste are adopted in some of the developed countries. Non-incineration technology comprises of shredding and disinfection by autoclaving/microwaving or chemical treatment. The treated waste can be disposed along with municipal solid waste in sanitary landfills or through waste to energy plants. Such option can also be adopted in places where the sanitary landfill or waste to energy plant for disposal of municipal

solid waste is available. Such technology is permitted only after prior approval of MoEF & CC and only after obtaining authorization under the BMWWM Rules from the respective SPCB/PCC for the purpose of carrying out trial runs for assessment of efficacy of the treatment equipment.

- j) *Vehicle/Containers washing facility:*** Every time a vehicle is unloaded, the vehicle and empty waste containers shall be washed properly and disinfected. Washing can be carried out in an open area but on an impermeable surface and liquid effluent so generated shall be conveyed and treated in an effluent treatment plant. The impermeable area shall be of appropriate size so as to avoid spillage of liquid during washing.
- k) *Effluent Treatment Plant:*** A suitable Effluent Treatment Plant (ETP) shall be installed to ensure that liquid effluent generated during the process of washing containers, vehicles, floors etc. is treated and reused after treatment. Proper treatment of waste water shall be ensured in case of zero discharge by recirculation of treated waste water for scrubbing. *ETP may have treatment unit operations* comprising collection tank, O & G trap, chemical dosing cum mixing (Flash and slow), coagulation chamber, primary settling tank (s), biological treatment process, secondary settling tank, pressure filter and activated carbon filter, pH Correction tank (wherever recirculation of treated water is practiced) *so as to comply* with the liquid discharge standards stipulated under the Bio-medical Waste Management Rules, 2016. ETP may also have the following provisions:
- (i) separate 'energy meter' so as to know total consumption of electricity for operation of the machinery attached with the ETP.
 - (ii) pH meter so as to know pH level of treated water as well as pH level of treated water used for recirculated or recycling in APCD attached with the incinerator or any utility within the CBWTF.
 - (iii) A 'magnetic flow meter' should also be fitted at all the water supply extraction points of the CBWTF as well as the outlet to know the total wastewater treated for further end use or discharge in compliance to the BMWWM Rules.
 - (iv) Provision of 'press filter' to reduce the moisture content of the ETP Sludge or it may be dried in 'sludge drying bed'. After removal of moisture content or drying, same need to be disposed off in an environmentally sound manner depending upon the hazardous constituents present in it as per Hazardous and Other Waste (Management and Transboundary Movement) Rules, 2016.

In case, ETP sludge contains metal contents within the prescribed limits as per Hazardous & Other Waste (Management & Transboundary Movement) Rules, 2016, such ETP sludge shall be given to CBWTF for incineration or to hazardous waste treatment, storage and disposal facility (TSDF) for disposal in secured landfill.

Note:

- a) If any CBWTF desires to adopt any other technology other than referred under Schedule –I of the BMW Rules, may adopt new technology only with the prior approval from MoEF & CC and is also required to obtain authorization under the BMW Rules from the respective SPCB/PCC for carrying out trial run for assessment of efficacy of the new technology.
- b) All the treatment equipment should be operated and complied with the norms as stipulated under Schedule II of the Bio-medical Waste Management Rules, 2016 published by MoEF & CC vide GSR 343 (E) dated 28th March, 2016.
- c) Incinerator / Plasma Pyrolysis/ Autoclaving/Microwaving/ Hydroclaving/ Shredder/ Dry Heat Sterilization/ ETP should be fitted with separate 'energy meter' for recording total energy consumed for operation of these equipment.
- d) In the event of temporary shutdown (not more than a week) due to any operational problems in the treatment equipment (such as restoration of refractory lining or maintenance or repairs in APCD), to ensure bio-medical waste collected from the member health care facilities is treated within the time limit as stipulated under the BMW Rules, each all the CBWTF operators should also be provided with stand by treatment equipment especially incinerator/plasma pyrolysis/autoclave (or) alternately MoU made with the nearby CBWTF (located within the State/UT) shall be submitted to the respective SPCB/PCC, by all the existing CBWTF operators (whereas the upcoming facilities have to make such arrangement prior to commencement of the facility) so as to include such condition while granting authorisation under the BMW Rules, 2016 to the concerned CBWTF operators (vice-versa).

(10) Infrastructure set up

The CBWTF shall have enough space within it to install required treatment equipment, untreated and treated waste storage area, vehicle-parking, vehicle and containers washing area, Effluent Treatment Plant (ETP), administration room or staff room etc. The required area for CBWTF would depend upon the projected amount of bio-medical waste to be handled by it. A CBWTF shall have the following infrastructure:

a) Treatment Equipment Room

A separate housing may be provided for each treatment equipment at the CBWTF such as incinerator room, autoclave room, microwave room etc., as applicable. Each room shall have well-designed roof and walls. Such room shall be well ventilated and easy to wash. The floor and interior finishing of the room shall be such that chances of sticking/harboring of microorganisms are minimized. This can be attained by

providing smooth & fine floor and wall surfaces (to a height of 2 meter from floor) preferably of tiles. The number of joints in such surfaces shall be minimal. The equipment room shall also have a separate cabin, to supervise the operation of the equipment and to record the waste handling and equipment operational data attached to each equipment room. There shall be two waste storage rooms, one for storage of untreated waste and another for treated waste and may be located at a distance from each other. The storage room shall have provisions similar to that of equipment room being well-ventilated with easy to wash floors & walls, smooth and fine surfaces etc. All the treatment equipment rooms and waste storage rooms should be provided with 'fly catcher/killing device'. The room shall be washed and cleaned with a suitable disinfectant every day.

b) Main waste storage space

Separate space shall be provided near the entry point of the CBWTF to unload and store all biomedical wastes that have been transported to the CBWTF by its own transportation vehicle. The size of the room shall be adequate to store all wastes transported to the CBWTF. The front portion of the room shall be utilized for unloading the wastes from the vehicle and back or side portion shall be utilized for shifting the wastes to the respective treatment equipment. In the front portion of the room where transportation vehicle is parked for unloading, the floor shall be made impermeable so that any liquid spillage during unloading does not percolates into the ground. The liquid generated during handling of wastes and washing, shall be diverted to the inlet of effluent treatment plant (ETP). In the main storage room, wastes shall be stacked with clear distinction as per the color coding of the containers by providing partitions. From here, the colored containers may be sent to the respective treatment equipment by using suitable closed type of conveyance (trolley etc.). The main storage room too shall have provisions similar to that of equipment room such as roofing, well ventilated, easy to wash floors & walls, smooth and fine surfaces etc.

Apart from the above, a CBWTF should have separate storage provision for storage of mercury bearing waste collected from the member health care facilities as per the procedure given in CPCB guidelines. Mercury storage provision should be provided as per the guidelines issued by CPCB (refer www.cpcb.nic.in). The capacity of the mercury storage provision should be maximum of 90 days and by which the collected mercury bearing waste shall have to be disposed of through a TSDF located nearby following the manifest as per Hazardous and Other Waste (Management and Transboundary Movement) Rules, 2016. The charges for collection and disposal of

mercury bearing waste shall be collected by the CBWTF from the respective member HCF.

c) Treated waste storage room

Separate space should be provided to store the wastes treated in different treatment units. The wastes shall be stored in separate group as per the disposal options. Other provisions in the room shall be similar to the main storage room. Waste such as incineration ash/vitrified ash generated in the process of incineration/plasma pyrolysis respectively shall be stored safely in a separate area under the shed so as to avoid entry of rain water during the monsoon and for easy collection. In case, incineration ash/ vitrified ash is found to be hazardous waste in nature same should be disposed of through any authorized TSDF operator located nearby following the manifest as per Hazardous and Other Waste (Management and Transboundary Movement) Rules, 2016. In case of a State/UT where TSDF is not available, all the CBWTF operators have to store incineration ash safely as per these guidelines.

d) Administrative Room

This room shall be utilized for general administration, record keeping, billing etc.

e) Generator set

CBWTF shall have a generator set of adequate capacity as standby arrangement for power, with sufficient capacity to run the treatment equipment during the failure of power supply. The generator set shall comply with the necessary requirement as per DG Set norms notified under the Environment (Protection) Act, 1986.

f) Continuous emission monitoring system (CEMS)

Monitoring provision for continuous monitoring of the incinerator/plasma pyrolysis stack emission shall be installed by the CBWTF operators for the parameters as stipulated by the respective SPCB/PCC as per the authorisation granted under the BMW Rules, 2016. Other-wise, at present, all the existing CBWTF operators are required to carry out stack emission monitored using continuous emission monitoring system for the flue gas parameters such as CO₂, O₂, CO as well as primary & secondary chamber temperatures, and records maintained. The continuous emission monitoring system for stack emission should be installed as per the guidelines issued by SPCB/PCC/CPCB. Also, the real time continuous stack emission

monitoring data is also required to be transmitted to the servers of the respective SPCB/PCC as well as CPCB, by all the existing CBWTF operators

g) Vehicle Parking

Provision for parking shall be made within the confines of the site for parking of required number of vehicles, loading and unloading of the vehicles meant for transporting waste to and from the facility, etc.. In case of a CBWTF with space constraints, multi-storey parking or a separate provision may be allowed only for parking of vehicles.

h) Display and sign board

An identification board (Display) of durable material and finish shall be displayed at the entrance to the facility. This shall clearly display the name of the facility, owner name, address and telephone number of the operator and the prescribed authority, no. of hours of operation & operational hours, telephone numbers of the personnel to be contacted in the event of an emergency, validity period of authorization as well as total daily waste treated and disposed. Also, sign boards should be provided at all the salient points (untreated waste storage area, treatment equipment, treated waste storage area, ETP, firefighting equipment) within the facility.

i) Washing Room

A washing room shall be provided for eye washing/hand washing/ bathing etc. for the workers.

j) Site Security

High walls, fencing and guarded gates shall be provided at the facility to prevent unauthorized access to the site by humans and livestock.

k) Fire safety

Fire safety equipment such as sand buckets and fire extinguishers should be provided at all the salient points of the CBWTF including at the diesel storage areas, diesel tanks connected with the incinerator etc. Fire alarm also should be provided within the CBWTF to prompt the workers in the event of any fire hazard. Workers should also be trained in First Aid administration.

l) First Aid Box

First Aid Box with necessary provisions need to be provided at all the salient points within the facility.

m) Green Belt

The open area available within the CBWTF shall be developed into green belt.

n) Website: (newly added as per BMWM Rules, 2016)

All the existing CBWTFs shall develop own website by 27.03.2017 whereas the upcoming CBWTF shall develop the website prior to the commencement of the facility. The website should be uploaded with relevant information periodically (on monthly basis) especially as detailed below:

- (i) A copy of the Environmental Clearance obtained;
- (ii) Copies of the Consents under the Water (Prevention and Control of Pollution) Act, 1974 and Air (Prevention and Control of Pollution) Act, 1981 as well as the Authorisation under the BMWM Rules obtained from the SPCB/PCC;
- (iii) List of all the member Health Care Facilities with complete address, bedded or non-bedded HCFs, no. of beds, bar code, category-wise average bio-medical waste generation in kg/annum;
- (iv) Charges levied on the member Health Care Facilities (HCFs) for treatment and disposal of bio-medical waste;
- (v) Vehicles connected with a provision of GPS as per BMWM Rules and Vehicle-wise route chart for collection, transportation of bio-medical waste from the member HCFs;
- (vi) Real time continuous online stack emission monitoring data;
- (vii) Daily bio-medical waste collected, received and treated (Member HCF-wise);
- (viii) Monthly details of total waste collected from the member HCFs, total waste treated, and treated recyclable plastic waste or glass waste sold to the parties and final mode of disposal of incineration ash;
- (ix) A copy of the annual report submitted to the respective SPCB/PCC;
- (x) Monitoring results of the stack emissions, treated wastewater and incineration ash, as per the frequency stipulated under the BMWM Rules;
- (xi) List of HCFs (located within the coverage area) with complete address which have not taken membership of the CBWTF for disposal of Bio-medical waste;
- (xii) Contact person, contact telephone number and e-mail addresses of the facility; and.

- (xiii) Provision to have access to the SPCB/PCC/CPCB/MoEF & CC/MoH & FW especially on GPS, online monitoring system and the data.

Besides the provisions suggested in the earlier paras, following important provisions should also be made in a CBWTF:

- (i) A telephone shall be provided and maintained at the facility.
- (ii) A First Aid Box shall be provided and maintained at the CBWTF.
- (iii) Proper lighting shall be provided at the facility.
- (iv) Proper care shall be taken to keep the facility and surroundings free from odors.
- (v) Measures shall be implemented to control pests and insects at the site.
- (vi) Measures shall be implemented to control the escape of litter from the site.
- (vii) Necessary provision shall be made to prevent and control noise generated, if any, due to the activities at the site.
- (viii) Necessary protective gear for the waste handlers shall be provided.
- (ix) Immunization to all the workers of CBWTF against all the diseases including especially Tetanus and Hepatitis -B as stipulated under the BMW Rules.
- (x) Workers should have provisions such as washing, toilet, and suitable place for eating.
- (xi) Workers should also be provided with N-95 mask besides other PPEs such as hand gloves, gumboots, goggles etc.

Every CBWTF operator shall submit a work-plan to the Prescribed Authority. The work-plan should include the details of facilities at the CBWTF, collection, transportation & storage of the bio-medical wastes, operational details etc.

11) Record keeping

Maintenance of records for all operations carried out at the CBWTF is very important to monitor overall operation of the CBWTF. It also helps in submission of the required information to be submitted to the 'Prescribed Authority' by 30th June of every year as per the format prescribed under the BMW Rules or provided by the SPCB/PCC. A well-maintained record of all the activities at the CBWTF also enables the facility operator to produce all information of the activities on demand of the concerned prescribed authority. The record should include all information relating to each activity at the CBWTF site as per BMW Rules which include accidents occurred (spills, injury, fire accident) and the measures taken and also, however, minimum requirement is outlined below:

a) Records of waste movements

Daily records shall be maintained for the waste accepted and treated waste removed from the site. This record shall include the following minimum details:

- (i) **Waste accepted:** -Records on day-to-day basis (as per the format given at **Annexure-II**) shall be maintained with respect to the waste collection date, name of the healthcare unit with bar code, waste category as per BMWWM Rules, category-wise quantity of waste accepted, vehicle registration number used for collection of bio-medical waste from member health care facilities, time at which waste collected from member HCFs, name of the vehicle driver and his signature and waste receiving date & time (at CBWTF site). Similar information to be acknowledged to the member health care facility by the CBWTF operator on daily basis.
- (ii) **Treated waste to be disposed:-** Date, treated waste type, Quantity, vehicle number, disposal as stipulated under BMWWM Rules.

b) Logbook for the treatment equipment

A logbook shall be maintained for each treatment equipment installed at the site and shall include the following:

- (i) The weight of each batch.
- (ii) The categories of waste as per the Rules.
- (iii) The time, date and duration of each treatment cycle and total hours of operations.
- (iv) The complete details of all operational parameters during each cycle.

Log book to be maintained for operating the incinerator/plasma pyrolysis as well as the autoclave as per the formats given at **Annexure –III.**

c) Monitoring and reporting of operations in the CBWTF:

The monitoring of the key operating parameters of treatment equipment provides several benefits. First, monitoring provides the operator with information needed to make decisions on necessary combustion control adjustments. Second, properly maintained monitoring records can provide useful information for identifying operating trends and potential maintenance problems. Following are the suggested parameters for monitoring of the treatment equipment

(i) Monitoring of operating parameters of the incinerator/plasma pyrolysis:

Following operating parameters can be monitored in case of incinerator/plasma pyrolysis:

- Waste charge rate.
- Combustion gas temperature in primary and secondary chamber as well as the temperature of the stack exit gas (flue gas).
- Condition of the draft (negative draft in primary chamber).
- Combustion gas oxygen level in primary and secondary chamber as well as stack exit gas.
- Air flow rate through the incinerator/plasma pyrolysis.
- Carbon-Di-Oxide (CO₂), Oxygen (O₂) and Carbon Monoxide (CO) level in the flue gas.
- Quantity of auxiliary fuel usage as well as the power consumption (in every batch).
- Pressure drop in the primary chamber and APCD attached with the incinerator/plasma pyrolysis and
- Bottom ash or slag quality (for Total Organic Carbon (TOC) as well as loss on ignition and the hazardous constituents (at least once in a quarter).

(ii) Monitoring of operating parameters of the Autoclave: Following operating parameters can be monitored during the sterilization using autoclave:

- Time at which sterilization started and time at which sterilization completed.
- Temperature conditions maintained throughout the sterilization
- Conditions of pressure maintained throughout the sterilization
- Duration of sterilization
- Validation test results

Records concerning the above parameters need to be maintained and checked periodically for taking remedial measures during the operation of the incinerator or plasma pyrolysis or autoclave. In case of other treatment processes, the operational conditions as well as the efficacy tests to be complied with as per the standards prescribed under the BMW Rules.

(iii) Frequency of monitoring:

The CBWTF operator shall carry out following tests through a NABL approved laboratory or a laboratory approved under the Environment (Protection) Act, 1986, as

per the frequency stipulated under the BMWWM Rules or as prescribed by the SPCB/PCC and record of such analysis results shall be maintained and submitted to the prescribed authority (SPCB/PCC), as suggested below:

- **Liquid effluent:** Parameters such as pH, Suspended Solids, Oil & Grease, BOD, COD, Bio-assay for liquid effluent being discharged from the CBWTF be monitored as per the Consent conditions or once in a quarter and such records maintained and submitted to SPCB/PCC.

- **Stack emission monitoring:**

In case of the BMW incinerators which came after 28.03.2016, the Stack Emission shall be monitored (under optimum capacity) for parameters such as Particulate Matter, HCl, NO_x, Hg & compounds and combustion efficiency *once in three months* as required under schedule II of the Bio-medical Waste Management Rules 2016 (All monitored values shall be corrected to 11% Oxygen on dry basis). In case of dioxins and furans, monitoring should be done *once in a year* (monitored values shall be corrected to 11% Oxygen on dry basis). In case of the incinerators (existing prior to the notification of BMWWM Rules, 2016), new incinerators standards are required to be complied within two years i.e., by 27.03.2018.

- **Validation test of autoclave/microwave/chemical treatment/dry heat sterilization:**

Suggested validation test for treatment of bio-medical waste by autoclave/microwave/chemical treatment/Dry heat sterilization is given in **Table 1**.

Table 1: Suggested validation test for treatment of bio-medical waste by autoclave/microwave/chemical treatment/Dry heat sterilization

S. No	Type of equipment used for treatment of bio-medical waste	Type of Validation Test	Frequency
(i)	Autoclave	(i) biological indicator strips or vials <i>Geobacillus stearothermophilus</i> spores with at least 1×10^6 spores),	once in three months
		(ii) chemical indicator strip or tape	each batch of waste treated
(ii)	Microwave	<i>Bacillus atrophaeus</i> spores using vials or spore strips with at least 1×10^4 spores per detachable strip	Recommended: once in three months
(iii)	Chemical treatment followed by shredding	<i>Bacillus Subtilis</i> (ATCC 19659)- 4 Log ₁₀ reduction or greater	Once in a week
(iv)	Dry heat sterilisation	consistently kill the biological indicator <i>Geobacillus Stearothermophilus</i> or <i>Bacillus Atropheaus</i> spores using vials with at least 6 log ₁₀ spores per ml.	Once in three months
		A chemical indicator strip or tape	Once in a week

d) Site Records:

Site records shall include the following:

- (i) All the approvals obtained from other concerned departments other than the prescribed authority;
- (ii) Details of construction or engineering works;
- (iii) Maintenance schedule, breakdowns/trouble shootings and remedial actions;
- (iv) Emergencies;
- (v) Incidents of unacceptable waste received and the action taken; and
- (vi) Details of site inspections by the officials of the regulatory authorities, purpose of visits with date and necessary actions initiated on the observations.

Daily, monthly and annual summary records of all the above shall be maintained and made available at the site for inspection and same submitted whenever required by an authorized official of the concerned regulatory authorities.

12) Collection and transportation of bio-medical waste

The collection and transportation of bio-medical waste shall be carried out in a manner so as to prevent any possible hazard to human health and environment. Collection and transportation are the two operations where the chances of segregated bio-medical waste coming in contact with the public, rag pickers, animals/birds, etc. are high. Therefore, all care shall be taken to ensure that the segregated bio-medical waste handed over by the healthcare units reach CBWTF without any damage, spillage or unauthorized access by public, animals etc. A responsible person from the CBWTF operator shall always accompany the vehicle to supervise the collection and transportation of bio-medical waste. Also, the private transport vehicles should not be authorised by the SPCBs/PCCs only for transportation of the Bio-medical Waste. The CBWTF operator should be made responsible for collection and transportation of bio-medical waste.

a) Collection of bio-medical waste:

Generator of the bio-medical waste is responsible for providing segregated waste in accordance with the provisions of the Bio-medical Waste Management Rules, 2016, to the CBWTF operator. Dedicated temporary storage at healthcare unit shall be designated. The coloured bags handed over by the healthcare units shall be collected in similar coloured containers with proper cover. Each bag shall be labeled as per Schedule IV of the Bio-medical Waste Management Rules as well as with bar coding system (to be complied by the occupier or operator of a CBWTF as per BMWM Rules) so that at any time, the healthcare units can be traced back that are not segregating the bio-medical wastes as per BMWM Rules. The coloured containers should be strong enough to withstand any possible damage that may occur during loading, transportation or unloading of such containers. These containers shall also be labeled as per Schedule IV of the Rules. Sharps shall be collected in puncture resistant container. The person responsible for collection of bio-medical wastes shall also carry a register with him to maintain the records such as name of the healthcare unit, the type and quantity of waste received, time at which waste collected from the member HCF, signature of the authorised person from the healthcare unit etc. During transportation, the containers should be covered in order to prevent exposure of public to odours and contamination.

(b) Transportation of the collected bio-medical waste to the CBWTF:

All the vehicles used by the CBWTF operator shall not be sub-letted or contract vehicles should not be used by the CBWTF operator. All the vehicles owned by the CBWTF operator and intended only for collection of bio-medical waste from the member health care facilities should be registered under the Motor Vehicle Act with the respective RTO/Transport Department and such vehicle numbers should also be registered with the respective SPCB/PCC for the purpose of collection of bio-medical waste from the member health care facilities. The bio-medical waste collected in designated coloured containers shall be transported to the CBWTF in a fully covered vehicle. Such vehicle shall be dedicated for transportation of bio-medical waste only. Depending upon the volume of the wastes to be transported, the vehicle may be a two or three-wheeler, light motor vehicle or heavy duty vehicle. In either case, the vehicle must possess the following:

- (i) Transportation vehicle shall be fitted with GPS to track the movement of the vehicle.
 - (ii) Separate cabins shall be provided for driver/staff as well as for placing the designated colour coded bio-medical waste containers.
 - (iii) Two wheeler registered under the Motor Vehicle Act shall be permitted for collection of bio-medical waste only from the clinics or dispensaries located in places where the lanes are narrow and not easily accessible to four wheeler vehicles. Such two wheeler vehicle (s) should have a provision of a suitable fixed waste collection box marked with bio-hazard symbol, contact details, proper lid, emergency spill collection procedure, first aid box and manifest record in accordance with the BMWWM Rules
 - (iv) The base of the waste cabin shall be leak proof to avoid pilferage of liquid during transportation.
 - (v) The waste cabin may be designed for storing waste containers in tiers and also should be provided with a lighting provision.
 - (vi) The waste cabin shall be so designed that it is easy to wash and disinfect.
 - (vii) The inner surface of the waste cabin shall be made of smooth surface to minimize water retention.
-

-
- (viii) The waste cabin shall have provisions for sufficient openings in the rear and/or sides so that waste containers can be easily loaded and unloaded.
 - (ix) The vehicle shall be labeled with the bio-hazard symbol (as per Schedule IV of the BMW Rules) and should display the name, address and contact telephone and mobile number of the CBWTF.
 - (x) The vehicle driver should carry always valid registration of the vehicle obtained from the concerned transport authority and also carry valid 'pollution under control certificate' issued by the authorized certificate issuing agency.

Depending upon the area to be covered under the CBWTF, the route of transportation shall be worked out. The transportation routes of the vehicle shall be designed for optimum travel distance and to cover all member healthcare units of the CBWTF. The CBWTF operator should ensure online and real time tracking & monitoring provisions (GPS provision) should be given access with passwords to the SPCB/PCC and CPCB to cross check the movement of the transportation vehicles on any time by the SPCB/PCC/CPCB. As far as possible, the transportation shall be carried out during non-peak traffic hours. If the area to be covered is very large, a satellite station may be established to store the bio-medical waste collected from the adjoining areas. The wastes so stored at satellite station may then be transported to the CBWTF in a big vehicle. It shall be ensured that the total time taken from generation of bio-medical waste to its treatment, which also includes collection and transportation time, shall not exceed 48 hours.

13) Disposal option of solid waste generated from the CBWTF

Treated plastic waste, incineration ash, treated waste sharps and glass waste, Oil & Grease waste and ETP sludge are generally generated from the CBWTF from the treatment systems such as autoclaving/microwaving, incineration, chemical disinfection and effluent treatment plant respectively. The treated bio-medical waste shall be disposed as per the options suggested in the **Table 2** given below:

Table 2: Suggested Disposal option of solid waste generated from the CBWTF

Sl. No.	Treated Waste Category	Suggested Treatment and Disposal Options
1.	Plastic wastes after disinfection and shredding	Plastic waste should not be sent to landfill sites. Treated plastic waste to be (i) sent to registered or authorized recyclers (or) (ii) for energy recovery (or) (iii) for diesel or fuel oil recovery (or) (iv) for road making, whichever is possible.
2.	Disinfected Sharps (including needles and syringes) (i.e., Treatment by Autoclaving or Dry Heat Sterilization followed by shredding or mutilation combination of shredding cum autoclaving)	Encapsulation in metal container or cements concrete; (or) sent for final disposal to iron foundries (having consent to operate from the SPCBs/PCCs (or) sanitary landfill or designated concrete waste sharp pit.
3.	Incineration ash	Incineration ash (ash from incineration of any bio-medical waste) shall be disposed through hazardous waste treatment, storage and disposal facility (TSDF), if toxic or hazardous constituents are present beyond the prescribed limits as given in Schedule –II of the Hazardous and Other Waste Management & Transboundary Movement Rules or as revised from time to time.
4.	Other treated solid wastes like Glass waste	Disinfection (by soaking the washed glass waste after cleaning with detergent and Sodium Hypochlorite treatment) or through autoclaving or microwaving or hydroplaning and then sent for recycling.
5.	Oil & Grease	By Incineration
6.	ETP Sludge	After drying in sludge drying beds or removal of moisture content using 'Filter Press' and such ETP sludge shall be given to CBWTF for incineration or to the hazardous waste treatment, storage and disposal facility (HWTSDf) for disposal in Secured Landfill
7.	Hazardous Waste	Disposal through a TSDF located nearby following the manifest as per the Hazardous and Other Waste (Management & Transboundary Movement) Rules, 2016

14) Cost to be charged by the CBWTF Operator for the Health Care Facilities

Cost to be charged from the healthcare facilities plays an important role in financial viability and sustainable operation of a CBWTF project, for providing the best treatment services to the Health Care Units and for ensuring compliance to the BMWM Rules. The cost shall be so worked out that neither it becomes a monopoly of the CBWTF operator nor the interest of the CBWTF operator is overlooked. It is recommended that cost to be charged from the healthcare units, depending on the size, no, of beds and the distance from the location of the CBWTF and same shall be worked out in consultation with the concerned SPCB/PCC and the local Medical Association, keeping in view the following options:

- (a) In case of non-bedded health care units, fixed charges depending on the average quantity of waste generation per day, in case of the nursing homes/clinics/sample collection Centres /Dental Centres, dispensary, pathological laboratory, blood banks, and other non-bedded hospitals irrespective of their system of medicine including ayush hospitals.
- (b) In case of bedded hospitals, fixed charges per bed per day basis and based on the no. of beds for which consents under the Water Act, 1974/Air Act, 1981 and authorization granted under the BMWM Rules, by the prescribed authority

Note:

- (i) *Rates are required to be revised once in a year based on the Wholesale Price Index (WPI Index) or Consumer Price Index (CPI Index) (considering the prevailing market price especially in respect of the labour expenses, diesel prices, electricity, operating cost etc.,), by the State Advisory Committee in consultation with the concerned SPCB/PCC, local Medical Association and the representatives of the CBWTF Association*
- (ii) *The Health Care Facilities are required to ensure timely payments to the CBWTFs for ensuring timely treatment services in compliance to the BMWM Rules as well as agreement made with the concerned CBWTF Operator.*

15) Check list for development of CBWTF

The criteria for development of CBWTDF have been discussed in detail in the

Previous sections. However, to have at a glance check in developing CBWTF, checklist is reproduced for convenience and is annexed **(Annexure-IV)**.

16) Periodic inspection/monitoring or performance evaluation of the CBWTF

To have uniformity in performance evaluation of the CBWTF throughout the country, a check list for performance evaluation of the CBWTF for carrying out inspection/monitoring/compliance verification has been prepared and is annexed **(Annexure –V)**. All the prescribed authority (SPCB/PCC) shall inspect the CBWTF at least once in six months located in the respective State/UT and a copy of the inspection reports shall be submitted to CPCB and MoEF & CC along with a copy of the action taken for ensuring compliance to the BMW Rules and CPCB guidelines issued from time to time and also such information is required to be uploaded in SPCB/PCC website. CPCB shall carryout random inspection of the CBWTFs once in a quarter and any violations observed further actions shall be initiated by CPCB if required under the Environment (Protection) Act, 1986.

-- OO --

Annexure-I**Coverage area-wise gap analysis for assessing additional BMW treatment capacity requirement**

S. No	Coverage area (pl. indicate areas covered by a CBWTF in the State/UT)	No. of HCFs		No. of Beds covered	Total estimated BMW generation in Kg/day	Total existing treatment capacity in Kg					Total BMW Treated and Disposed in Kg/day	Gap between total BMW Generation and the Existing BMW Treatment Capacity in Kg	Remarks (Whether additional Treatment Capacity is required or not)	
		Bedded	Non-bedded			Incineration	Autoclaving/ Hydroclaving /microwaving	Chemical disinfection	Deep burial	Any other mode of disposal			Yes	No
(1)	(2)	(3)	(4)	(5)	(6)	(7)	(8)	(9)	(10)	(11)	(12)	(13)	(14)	(15)

Note: Above gap analysis coverage area-wise is required to be prepared once in five years and should be shown or depicted in a Map of State/UT.

Annexure- II**Format for maintaining the records by the CBWTF Operator alongwith the transportation Vehicle used for collection of bio-medical waste from the member HCFs**

Name of the CBWTF :
 Address of the CBWTF with contact details :
 Vehicle Registration Number (certificate to be carried by the vehicle driver) :
 Route covered (indicate places) by the vehicle :

Date	Vehicle number and the Time of arrival of the vehicle	Vehicle Speedo meter mileage readings in KM		Name of the HCF with address and the bar code number from whom waste collected	Category-wise quantity of bio-medical waste received in kg					Total BMW collected by the CBWTF		Name of the Vehicle driver with	Signatures	
		Initial	Final		Yellow	Red	Blue	Out dated medicines	White-Waste Sharps				Vehicle Driver	Representative of the HCF
										Total No. of Bags	Total waste			
(1)	(2)	(3)	(4)	(5)	(6)	(7)	(8)	(9)	(10)	(11)		(12)	(13)	(14)

Note: Above format is required to be maintained in duplicate both by the CBWTF Operator and the member HCF

Log book for Operating the Incinerator/Plasma Pyrolysis

[illegible]

Note: Fill the details whichever is applicable

Log Book for Operating the Autoclave/Hydroclave

[illegible]

Annexure – IV

Check List for Development of a Common Bio-medical Waste Treatment and Disposal Facility & For issuing 'Consent to Establishment under Water & Air Acts

-
1. Name of the Proponent :
 2. Proposed location of the CBWTF :
 3. No. of HCFs in the locality :
 4. No. beds :
 5. Total Bio-medical Waste Generation in kg/day :
 - (i) Incinerable in kg/day :
 - (ii) Autoclavable in kg/day :
 - (iii) Glass waste in kg/day :
 - (iv) Waste sharps in kg/day :
 6. **Proposed location of the CBWTDF:** located away from
 - a) Residential area : Yes ☐ No ☐
 - b) Sensitive area : Yes ☐ No ☐
 - c) Industrial area : Yes ☐ No ☐
 - d) Is it as a part of TSDF : Yes ☐ No ☐
 - e) Is the facility proposed in Hilly areas : Yes ☐ No ☐
 - d) Buffer distance of 500 m available : Yes ☐ No ☐
 7. **Proposed land area for CBWTF:**
 - a) Area about 1 acre : Yes ☐ No ☐
 - b) Area less than 1 Acre : Yes ☐ No ☐
 - c) Area more than 1 Acre : Yes ☐ No ☐
 8. **Proposed coverage area of the CBWTF:**
 - a) Any facility located upto a radius of 75 KM from the proposed locality : Yes ☐ No ☐
 - b) No. of beds covered by the existing facility/proposed facility:
 - (i) more than 10, 000 beds : Yes ☐ No ☐
 - (ii) less than 10,000 beds : Yes ☐ No ☐
 - c) Is there any CBWTF within the radius of 75 KM : Yes ☐ No ☐
 - d) BMW Waste generation in a coverage area under consideration: Kg/day
-

- e) Existing CBWTF treatment Capacity :
 (a) Incineration/plasma pyrolysis : Kg/day
 (b) Autoclave/hydroclave :Kg/day
 f) Is locality requires any additional capacity (within a radius of 75 KMs)?.
 : Yes ☐ No ☐
 (i) If so, indicate reason:.....

9. Requirement of Treatment Facility: Following treatment facilities shall be provided in a CBWTF:

- a) Incineration : Yes ☐ No ☐
 b) Autoclave (Pre-vacuum horizontal feeding) / Hydroclave / Microwave.
 : Yes ☐ No ☐
 c) Shredder : Yes ☐ No ☐
 d) Sharp pit (with drawing details) : Yes ☐ No ☐
 e) Provision for floor washing/vehicle washing: Yes ☐ No ☐
 f) Effluent Treatment Plant : Yes ☐ No ☐
 g) Secured land fill/Disposal of ash in TSDF : Yes ☐ No ☐
 h) Other provisions as per CPCB guidelines : Yes ☐ No ☐

10. Segregation

- (i). Segregation shall be as per the Bio-medical Waste Management Rules, 2016 as amended as well as compatible with treatment facilities at CBWTF
 (ii). Occupier/Generator is responsible for providing segregated waste to the operator.

11. Collection

- (i) Respective coloured bags provided with bar code should be kept in similar coloured container i.e. coloured bags shall not be directly kept in vehicle.
 (ii) Sharps shall be collected in puncture resistant, leak proof, rigid containers.
 (iii) Temporary storage at healthcare unit shall be designated.

12. Transport Vehicle

- (I) Dedicated vehicles for collection of Bio-medical waste : Yes ☐ No ☐
 (II) Separate cabins shall be provided for driver/staff and the
 bio-medical waste containers : Yes ☐ No ☐

- (III) The base of the waste cabin shall be leak proof to avoid pilferage of liquid during transportation : Yes ☐ No ☐
- (I) The waste cabin may be designed for storing waste containers in tiers : Yes ☐ No ☐
- (V) The waste cabin shall be so designed that it is easy to wash and disinfect. : Yes ☐ No ☐
- (VI) The inner surface of the waste cabin shall be made of smooth surface to minimize water retention : Yes ☐ No ☐
- (VII) The waste cabin shall have provisions of sufficient openings in the rear and/or sides so that waste containers can be easily loaded and unloaded : Yes ☐ No ☐
- (VIII) The vehicle shall be labeled with the bio-hazard symbol (as per Schedule IV of BMW Rules) and should display the name, address and telephone number of the CBWTF : Yes ☐ No ☐
- (IX) Other provision as per CPCB guidelines : Yes ☐ No ☐

13. Storage

- (I) Sufficient ventilated storage space for untreated and treated bio-medical waste shall be provided. : Yes ☐ No ☐
- (II) The flooring and walls (to a height of 2M from floor) shall be finished with smooth and fine material. There shall be minimum number of joints. : Yes ☐ No ☐

14. Record Keeping

- (I) Documents such as collection advice taken from health care units for each category of waste, records of waste movements, logbook for the equipment and site records shall be maintained. : Yes ☐ No ☐
- (II) All the record (five year) shall be available at the CBWTF site for inspection. : Yes ☐ No ☐

15. Proposed Treated Waste Disposal method:

- (i). Incineration ash - Secured landfill/near by TSDF : Yes ☐ No ☐
- (ii). Plastic waste after disinfection and shredding –Registered Recycling Unit : Yes ☐ No ☐
- (iii). Sharps, after disinfection (if encapsulated) - Municipal landfill : Yes ☐ No ☐
- (iv). Treated wastewater –Discharge into sewer/drain or recycling in APCD

- (v). Oil & grease –By incineration: : Yes ☐ No ☐
- (VI). Any other mode of disposal of recyclable waste: : Yes ☐ No ☐
- (If so, pl. indicate)

16. Estimated energy consumption and fuel consumption per month :

- (i) Estimated energy consumption per month
- (a) General lighting in the facility :
- (b) Incinerator :
- (c) Autoclave/microwave :
- (d) Shredder :
- (e) ETP :
- (f) Any other :
- (ii) Estimated fuel consumption:
- (a) Diesel consumption :..... in Kl per month
- (b) No. of hours of operation of DG Set :
- (c) No. of hours of incineration :

17. Whether the proponent obtained necessary approvals from the concerned departments as required : Yes ☐ No ☐

(i) If yes, attach details

18. Whether the proponent obtained EC as per EIA 2006 and the amendments made thereof : Yes ☐ No ☐

(i) If yes, attach a copy of the EC obtained from the concerned

19. Whether the proposal recommended for issuing consent to establish

: Yes ☐ No ☐

(Signature of the official verified with date)

Annexure – V

**Check List for Performance Evaluation of the
Common Bio-medical Waste Treatment and Disposal Facility (CBWTF)**

S.No.	Details		Particulars
01.	Name of CBWTF with contact details	:	
02.	Date of visit	:	
03.	Location details of the CBWTF	:	a) Near to Residential area: :Yes ☐ No ☐ b) In/near Sensitive area: Yes ☐ No ☐ c) In Industrial area : Yes ☐ No ☐ d) Is there a buffer zone of 500 m: Yes ☐ No ☐ Indicate exact distance: in KM e) Is it as a part of TSDF: Yes ☐ No ☐ If so, distance of TSDF from the nearest CBWTF:KM.. f) Is the facility proposed in Metropolitan city: Yes ☐ No ☐ (i)Name of the City: (ii)Population of the City (as per latest census): g) Is the facility proposed in Hilly area : Yes ☐ No ☐ (i)Name of the Town/City:
04	Month / year of establishment and the Consents status	:	Establishment Month/Year :
05.	CBWTF set up by	:	
06.	CBWTF operated by	:	
07.	Total number of healthcare facilities and beds covered (as on date of visit)	:	No. of HCFs : No. of Beds : No. of HCFs and beds upto 75 KM radius:
08.	Total BMW Treatment Capacity of CBWTF (in kg / day)	:	Incineration : Autoclave : Any other treatment and disposal:

S.No.	Details	Particulars
09.	Consents and Authorization details :	
9.1	Consent under Water (Prevention and Control of Pollution) Act, 1974	: ☐ Applied for ☐ Not Applied for ☐ Possess Valid Consent ☐ Not renewed ☐ No consent If obtained: Consent is valid upto and issued bySPCB/PCC vide letter dated
9.2	Consent under Air (Prevention and Control of Pollution) Act, 1981	: ☐ Applied for ☐ Not Applied for ☐ Possess Valid Consent ☐ Not renewed ☐ No consent If obtained: Consent is valid upto and issued bySPCB/PCC vide letter dated
9.3	Environmental Clearance (EC)	: ☐ Applied for ☐ Not applied ☐ Obtained ☐ Not obtained If obtained: EC issued by SEIAA or MoEF& CC vide letter dated
9.4	Authorization under BMW Rules, 1998	: ☐ Applied for ☐ Not Applied for ☐ Possess Valid Authorisation ☐ Not renewed ☐ No Authorisation If obtained: Authorisation is valid upto and issued bySPCB/PCC vide letter dated
10.	Investment in setting up the CBWTF	:
11.	Area of plot size for CBWTF (Sq. ft.)	:
12	Annual Report submission for the year	: Submitted before due date : :Yes ☐ No ☐ If yes, provide details of waste collected, received and treated & disposed of:
12.	Coverage area of CBWTF (radius in KM covered)	: Coverage area upto 75 km radius: Yes ☐ No ☐
13.	Name of Districts/Cities / places being covered	: (Pl. indicate Districts or places covered:.....)) W.r.to the CBWTF (i) Farthest HCF located at : ..KM (ii) Nearest HCF located at :.....KM.

S.No.	Details		Particulars
14.	Daily operation schedule (timings)	:	(i) Collection: ...AM to PM. (ii) Incineration:....AM toPM (iii) Whether waste from member HCFs collected in holidays: ☐ Yes ☐ No
15.	Cost charged to the healthcare facilities	:	(i) Charges in Rs..... (ii) Is the cost to be levied suggested by:Organisation
16.	Total quantity of bio-medical waste treated: kg/day (avg.)		
16.1	Incinerable	:	 %
16.2	Autoclaving	:	%
16.3	Others (please specify waste type-wise)	:	%
17.	Staff involvement in CBWTF operation (number of persons):		
17.1	Managerial / Administration	:	
17.2	Equipment operations	:	
17.3	Transportation of BMW	:	No. of Drivers: No. of Helpers:
17.4	Sanitation and others	:	
17.5	Total persons excluding managers	:	
18.0	Collection and Transportation of bio-medical waste from member HCFs :		
18.1	No. of Vehicles used for collection of waste from member HCFs	:	(i) Four Wheelers:Nos and Vehicle Numbers: (ii) Two Wheelers :.....Nos and Vehicle Numbers:.....
18.2	Vehicles are labeled as per BMW Rules, 2016	:	☐ Satisfactory ☐ No satisfactory
18.3	Vehicles used are as per CPCB Guidelines	:	☐ Satisfactory ☐ No satisfactory
18.4	Vehicles attached with the GPS provision as per BMW Rules 2016	:	☐ Satisfactory ☐ No satisfactory
18.5	Whether waste collected from member HCFs adopted Bar coding system ?	:	☐ Yes ☐ No

S.No.	Details		Particulars												
19.0	Temporary untreated waste storage area	:	☐ Satisfactory ☐ No satisfactory												
20.0	Mode of conveyance of bio-medical waste from untreated waste storage area to the treatment equipment within the CBWTF	:	☐ Closed Trolley/Pull cart with bio-hazard symbol ☐ No Closed Trolley/Pull cart ☐ Others like												
21.0	Treatment equipment installed at CBWTDF														
21.1	Incinerator/plasma pyrolysis capacity and make	:	(i) No. of Incinerators including standby: (ii) Incineration capacity: kg /hrKg/day.												
21.2	Daily Operation schedule of the incinerator /plasma pyrolysis (timings)	:	AM toPM (or)PM toAM Whether bio-medical waste collected from member HCFs is treated during holidays: Yes ☐ No ☐												
21.3	Consumption of auxiliary fuels	:	<table border="1"> <thead> <tr> <th>S. No</th><th>Type of Fuel</th><th>Consumption Quantity in liters per day</th><th>Bill numbers of purchase of fuel</th></tr> </thead> <tbody> <tr> <td>a)</td><td></td><td></td><td></td></tr> <tr> <td>b)</td><td></td><td></td><td></td></tr> </tbody> </table>	S. No	Type of Fuel	Consumption Quantity in liters per day	Bill numbers of purchase of fuel	a)				b)			
S. No	Type of Fuel	Consumption Quantity in liters per day	Bill numbers of purchase of fuel												
a)															
b)															
21.4	Stack attached with the incinerator /plasma pyrolysis	:	(i) Stack Diameter: m (ii) Stack Height : m above Ground Level												
21.5	Monitoring provision attached with the stack	:	☐ Platform ☐ Porthole ☐ access to the platform (Steps/Monkey Ladder/any other.....)												
21.6	Is stack monitoring provision satisfactory and as per CPCB guidelines	:	☐ Yes ☐ No												
21.7	air pollution control systems attached with the incinerator/plasma pyrolysis	:	(i) Quenching : ☐ Yes ☐ No (ii) Venturi scrubber : ☐ Yes ☐ No (iii) Droplet separator : ☐ Yes ☐ No (iv) Mist eliminator : ☐ Yes ☐ No (v) Filters : ☐ Yes ☐ No (vi) Lime and Activated Carbon injection: : ☐ Yes ☐ No												

S.No.	Details		Particulars
			(vii) ID Fan : ☐ Yes ☐ No (viii) Any other : (Pl. indicate)
21.8	Waste feeding mechanism	:	(i) Manual feeding : ☐ Yes ☐ No (ii) PLC based Automatic feeding : ☐ Yes ☐ No
21.9	Is PLC and automatic recording system (for recording operating parameters of the incinerator) attached with the incinerator/plasma pyrolysis	:	(i) PLC synchronized with waste feeding mechanism & in working condition: ☐ Yes ☐ No (I) PLC synchronized and recording system attached with incinerator and in working condition: ☐ Yes ☐ No
21.10	Operational conditions of the Incineration/plasma pyrolysis as observed during the visit	:	(i) Whether burners in working condition: ☐ Yes ☐ No (ii) Temperature maintained in Primary Chamber (range) : ^o C (iii) Temperature maintained in Secondary Chamber (range):..... ^o C (iv) Negative draft in Primacy Chamber :mm of water column (v) Pressure drop in the Venturi: mm of water column
21.11	Is continuous on-line monitoring system/Flue gas analyser attached with the incinerator/plasma pyrolysis for flue gas analysis (i.e CO, O ₂ and CO ₂)	:	(i) Is continuous online monitoring system (COMS) attached with incinerator: ☐ Yes ☐ No (ii) Observed values of flue gas parameters: CO ₂ : : .%; O ₂ : : % and CO: : % (iii) Observed Combustion Efficiency: :% (iv) Observed values of stack emissions as per COMS :
21.12	Emergency and Fire safety measures adopted within the facility is adequate	:	Is Emergency stack attached with the incinerator: ☐ Yes ☐ No Whether fire safety measures adopted (Fire Extinguishers, Sand buckets etc.): ☐ Yes ☐ No
21.13	Log book for incinerator/ plasma pyrolysis is maintained and satisfactory	:	Log Book Maintained: ☐ Yes ☐ No Log Book Maintained is satisfactory : ☐ Yes ☐ No

S.No.	Details		Particulars
21.14	Details of heat recovery system installed with incinerator/plasma pyrolysis	:	☐ Yes ☐ No
22.0	Capacity of autoclave and-- make	:	Autoclave of capacitykg/cycle and make installed.
22.1	Operating conditions of autoclave/microwave as observed during the visit	:	Operating parameters observed: (i) Temperature : in °C (ii) Pressure : in psi (iii) Residence time : in minutes
22.2	Provision made for the autoclave /microwave	:	Trolley for waste feeding : ☐ Yes ☐ No Graphic or computer recording device attached: ☐ Yes ☐ No
22.3	Spore test or strip test conducted regularly and records maintained	:	☐ Yes ☐ No Pl. indicate frequency of Strip test conducted: every batch /once in a week /quarterly /yearly Pl. indicate frequency of Spore test conducted: every batch /once in a week /quarterly /yearly
22.4	Performance of autoclave by spore testing or routine test	:	☐ Satisfactory ☐ Not satisfactory
22.5	Log book maintained for autoclave is satisfactory	:	Log Book Maintained: ☐ Yes ☐ No Log Book Maintained is satisfactory : ☐ Yes ☐ No
23.0	Capacity of shredder and make	:	 kg/hr. Self-designed & got fabricated locally.
24.0	Details of sharp pit / Encapsulation facility	:	(i) Sharp Pit provided : ☐ Yes ☐ No (ii) Is it as per CPCB guideline : ☐ Yes ☐ No (iii) Records maintained : ☐ Yes ☐ No (iv) Total quantity of waste sharps stored: (v) Total quantity of waste sharps treated and disposed:
25.0	Water Balance		
25.1	Source and quantity of water intake per day (cu.m / day)	:	Water consumption source: Water is drawn at KLD approximately. Is magnetic water flow meter attached to the water source/water storage tank : ☐ Yes ☐ No

S.No.	Details		Particulars														
			Magnetic water flow meter readings as per record (for last month): 1st Day of Month : Last day of month : Magnetic Flow meter as observed during the visit: <table border="1"> <thead> <tr> <th rowspan="2">S. No</th><th rowspan="2">Month</th><th colspan="2">Magnetic flow meter reading</th></tr> <tr> <th>Initial</th><th>Final</th></tr> </thead> <tbody> <tr> <td>(1)</td><td>Previous month</td><td></td><td></td></tr> <tr> <td>(2)</td><td>On the date of visit:.....</td><td></td><td></td></tr> </tbody> </table> If water requirement is met from outside through tankers, pl. provide No. of Tankers procured in a previous six months: Total quantity of water consumed during the previous six months : in KLD	S. No	Month	Magnetic flow meter reading		Initial	Final	(1)	Previous month			(2)	On the date of visit:.....		
S. No	Month	Magnetic flow meter reading															
		Initial	Final														
(1)	Previous month																
(2)	On the date of visit:.....																
25.2	Break up of water usage (such as washing, scrubbing etc.)	:	Scrubber – KL/hr or KLD Washing – KLD Disinfections – KLD Gardening – KLD Domestic – KLD														
26.0	Total wastewater effluent generated per day	:	AboutKLD generated Quantity of treated water reused/recycled in %: Any other mode of disposal:														
27.	Effluent treatment plant details																
27.1	ETP Capacity	:	 KL/Cycle														
27.2	Flow Chart of ETP	:	ETP comprising of: Unit operations														
27.3	Intake and Discharge of ETP	:	(i) Magnetic Flow measuring device provided at the outlet of ETP: ☐ Yes ☐ No (ii) Energy meter attached to the ETP: ☐ Yes ☐ No (iii) Energy consumed over a period of one month: = Units (iv) pH meter attached at the outlet of ETP: ☐ Yes ☐ No														

S.No.	Details		Particulars
27.4	Final mode of disposal of treated water	:	(i) Is treated wastewater complying with the discharge norms ☐ Yes ☐ No (ii) Is Treated water is reused in the scrubber: ☐ Yes ☐ No (ii) Is Treated water is reused for gardening: ☐ Yes ☐ No (iii) Is Treated water is discharged in drain: ☐ Yes ☐ No (iv) Is Treated water is discharged in open area: ☐ Yes ☐ No
28.	Status of infrastructure provided (Pl. indicate 'Yes / No' whichever is applicable)		
28.1	Separate treatment equipment room	:	☐ Yes ☐ No
28.2	Main waste storage room	:	☐ Yes ☐ No
28.3	Treated waste storage room	:	☐ Yes ☐ No
28.4	Administrative room	:	☐ Yes ☐ No
28.5	Generator set	:	☐ Yes ☐ No
	(i) Capacity	:	
	(ii) Is Stack attached as per DG Set norms	:	☐ Yes ☐ No
	(iii) Is Acoustic enclosure provided as per DG Set norms	:	☐ Yes ☐ No
	(iv) Is DG Set complying to the emissions norms and noise level norms	:	☐ Yes ☐ No If so, pl. indicate latest monitoring results:
28.6	Site security (high walls, fencing, guarded gates etc.)	:	High walls on all four sides : ☐ Yes ☐ No Fencing on all the sides : ☐ Yes ☐ No Guarded Gates : ☐ Yes ☐ No Any other observation pl indicate:.....

S.No.	Details		Particulars
28.7	Parking facility	:	☐ Yes ☐ No
28.8	Sign board	:	☐ Yes ☐ No
28.9	Green belt	:	☐ Yes ☐ No
28.10	Washing room	:	☐ Yes ☐ No
28.11	First aid box	:	☐ Yes ☐ No
28.12	Lighting arrangements in the facility	:	☐ Yes ☐ No
28.13	Odour problem remedial measures	:	☐ Yes ☐ No
28.14	Fire fighting and emergency facilities	:	☐ Yes ☐ No
28.15	Measures for control of pests / insects etc.	:	☐ Yes ☐ No
28.16	Protective gear for waste handlers	:	☐ Yes ☐ No
28.17	Telephone facility	:	☐ Yes ☐ No
28.18	Provision of washing, toilets and safe place for eating for the workers		☐ Yes ☐ No
28.19	Fire alarm system provided in the facility		☐ Yes ☐ No
29.	Record maintenance and record keeping details (Pl. indicate 'Yes / No' whichever is applicable)		
29.1	Waste Movement /Manifest record	:	☐ Yes ☐ No
29.2	Log book for treatment equipment	:	☐ Yes ☐ No
29.3	Site records	:	☐ Yes ☐ No
29.4	Incineration ash generation and final disposal records	:	☐ Yes ☐ No
29.5	Treated plastic waste generation and its sale to the registered recycler	:	☐ Yes ☐ No
29.6	Syringes treated and its final disposal record	:	☐ Yes ☐ No

S.No.	Details		Particulars
29.7	Workers health status records		☐ Yes ☐ No
29.8	Workers immunization records		☐ Yes ☐ No
29.9	Medical and para-medical workers training records		☐ Yes ☐ No
29.10	Whether records maintained with regard to the accidents (such as fire, spills and injury and measures taken)		☐ Yes ☐ No
30.	Collection and transportation status (Yes / No)*		
30.1	Whether waste collected in a container of similar colour with label as per the Rules?	:	☐ Yes ☐ No
30.2	Whether the person who collects BMW maintain a register with him / her?	:	☐ Yes ☐ No
30.3	Has due attention have been given in vehicles to prevent spillage / pilferage/ loading / unloading etc.?	:	☐ Yes ☐ No
30.4	Is the vehicle labeled with the symbol and display the name, address, telephone number etc.?	:	☐ Yes ☐ No
30.5	Does the CBWTF operator use satellite station to store the waste?	:	☐ Yes ☐ No (If yes, give details.....)
30.6	The CBWTF operator collects waste daily or alternate day including	:	☐ Yes ☐ No


S.No.	Details		Particulars
	holidays?		
30.7	Whether waste treatment criterion of 48 hours is complied?		☐ Yes ☐ No
31.	Disposal of treated waste:		
31.1	Plastic waste after treatment	:	Plastic waste Sold to: M/s. and approved bySPCB/PCC
31.2	Treated sharps	:	Treated syringes disposal by:..... or through M/s.....and approved bySPCB/PCC
31.3	Incineration ash	:	Incineration ash disposal by: Disposal in Sanitary Landfill: ☐ Yes ☐ No Disposal through TSDF: ☐ Yes ☐ No Any other mode :.....
31.4	Other treated solid wastes	:	
31.5	Oil & grease	:	
31.6	Treated wastewater	:	
32.	Frequency of incinerator / autoclave / microwave / hydroclave / ETP discharge effluent testing and name of the laboratory (specify approved or not under E(P) Act, 1986 or NABL Accredited Lab.). Give details of compliance / non-compliance)	:	(i) Reported monitoring frequency: (ii) Stack monitoring : Quarterly : ☐ Yes ☐ No (iii) Waste water : Monthly/Quarterly/Yearly (iv) Incineration ash : Monthly/Quarterly/Yearly (v) Name of the Laboratory conducted test: (vi) Is the Laboratory approved under E (P) Act, 1986/.....SPCB/PCC/ NABL: : ☐ Yes ☐ No (vii) Copies of the analysis reports of treated effluent, incinerated ash, stack monitoring as (Annexures.....)
32.1	Frequency of site inspection by SPCBs/PCCs/CPCB/any other agencies	:	(i) No. of times in a year inspected by the SPCB/PCC: (ii) No. of times in a year inspected by the CPCB

S.No.	Details	Particulars																					
33.	Monitoring Results :																						
33.1	Incinerator stack emission (parameters stipulated in the Rules, temperature attainment in the chambers, residence time in the secondary chamber etc.)	<table border="1"> <thead> <tr> <th>Parameter</th> <th>PM</th> <th>HCl</th> <th>NOx</th> <th>Hg & compounds</th> <th>Dioxins and Furans</th> <th>C.E.</th> </tr> </thead> <tbody> <tr> <td>Date</td> <td></td> <td></td> <td></td> <td></td> <td></td> <td></td> </tr> <tr> <td>LIMIT</td> <td>50</td> <td>50</td> <td>400</td> <td>0.05</td> <td>0.1 ng TEQ per Nm³</td> <td>99.00%</td> </tr> </tbody> </table> Date of monitoring: Note: All values are in mg/Nm³, except CE	Parameter	PM	HCl	NOx	Hg & compounds	Dioxins and Furans	C.E.	Date							LIMIT	50	50	400	0.05	0.1 ng TEQ per Nm ³	99.00%
Parameter	PM	HCl	NOx	Hg & compounds	Dioxins and Furans	C.E.																	
Date																							
LIMIT	50	50	400	0.05	0.1 ng TEQ per Nm ³	99.00%																	
33.2	Whether Stack emission norms are complied with by the CBWTF	☐ Yes ☐ No																					
33.3	Incineration ash characteristics	Characteristics as per Schedule –II of HOW (M&TM) Rules,2016 (Annexure-----) Is it hazardous waste as per HOWM&TM Rules, 2016: ☐ Yes ☐ No																					
33.4	ETP inlet/outlet characteristics	All values are in mg/l except pH <table border="1"> <thead> <tr> <th>Parameter</th> <th>pH</th> <th>TSS</th> <th>COD</th> <th>BOD</th> <th>O&G</th> </tr> </thead> <tbody> <tr> <td>ETP Inlet Result</td> <td></td> <td></td> <td></td> <td></td> <td></td> </tr> <tr> <td>ETP Outlet Result</td> <td></td> <td></td> <td></td> <td></td> <td></td> </tr> </tbody> </table>	Parameter	pH	TSS	COD	BOD	O&G	ETP Inlet Result						ETP Outlet Result								
Parameter	pH	TSS	COD	BOD	O&G																		
ETP Inlet Result																							
ETP Outlet Result																							
33.5	Whether liquid effluent discharge norms are complying by the CBWTF	☐ Yes ☐ No																					
33.6	Whether CBWTF is submitting the annual report within the due date for the preceding year	☐ Yes ☐ No If Yes, annual report submitted vide letter No..... dated.....																					
34.	Any other relevant observations	(pl. enclose as annexure)																					
35.	Name of the officials with designation inspected /monitored the CBWTF and the signature																						

Annexure-VI

STATIONARY SOURCE EMISSION MONITORING

MODIFICATIONS TO BE MADE TO SAMPLING PLATFORM AND SAMPLING PORT HOLE

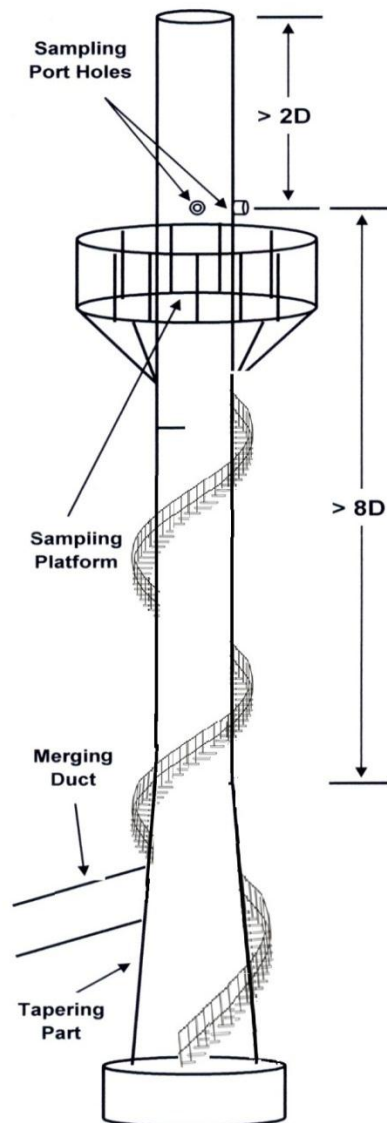


Number of Port Holes : Minimum two numbers of Port Holes at 90° apart from each other at a horizontal plane.

Location of Port Holes : Minimum 8 times of Internal Diameters of Stack downstream (upward direction of stack) from any duct confluence, bends and tapering & minimum 2 times of Internal Diameters of Stack upstream (downward direction of stack) from stack exit.


Location of Sampling Platform : 5 feet upstream (downward direction of stack) from the Port Hole as determined above.

Port Hole Flange : If the internal diameter of the flange is 4 inch or more then there is no need to change, if it is less than 4 inch then it has to be replaced with 4 inch flange. The flange should not protrude out more than 6 inches from the outer wall of the stack (it shall be kept as less as possible).


Sampling Platform Modification : A semi-circular extension of the existing platform (width extending outward by 6 feet from outside wall of the stack and covering at least one third of the circumference) may be provided for access to both the Port Holes. This area can be extended from the existing Platform and if deemed necessary for safety of the personnel a counter extension in opposite direction may also be provided. The extended Platform shall be strengthened with requisite support from the stack.

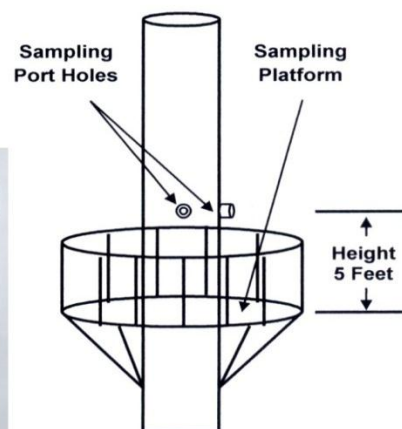


Note: Alternatively, safe access to monitoring platform may be provided with separate scaffolding-cum-staircase arrangement

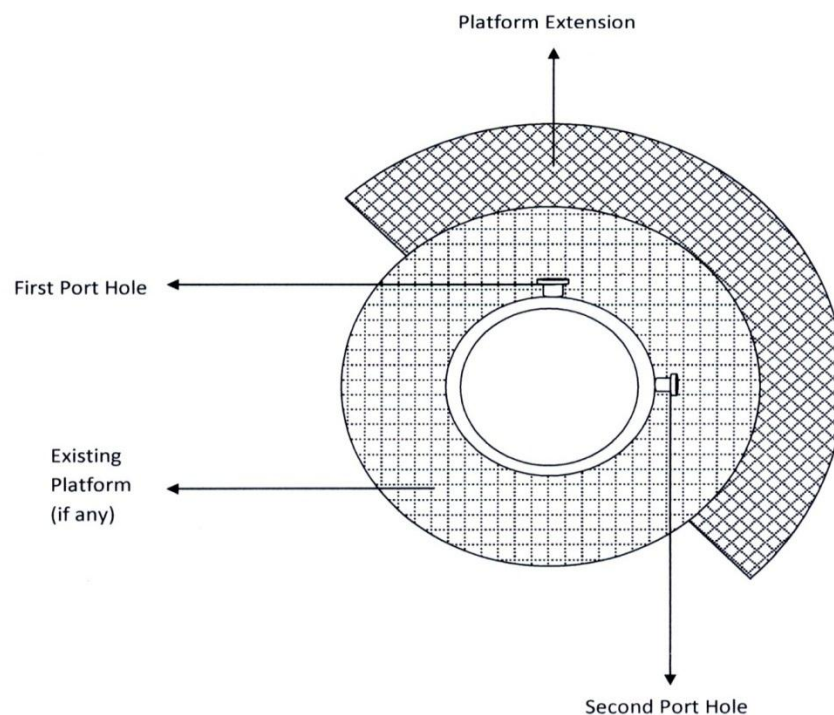

Sampling Platform Modification / Extension

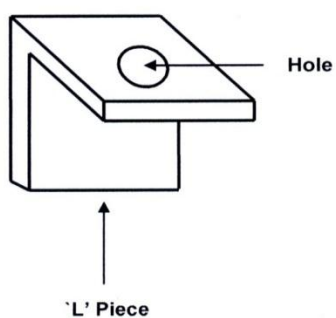

Fixing of 'L' Pieces on the stack wall : Two 'L' shaped pieces are to be fixed on the stack wall for mounting the Mono-Rail & Chain (part of the Sampling Kit for movement of sampling Train in & out through the Sampling Port Hole). The 'L' pieces shall be made of approximately 6 mm thick galvanized iron to have 5 cm long arms. One arm of the 'L' piece shall be welded on the stack wall and another arm shall have a hole of 14 mm diameter near the open end. Both the 'L' Pieces shall be welded on the stack wall at specified distances (as shown in the diagram on the next page) from the centre of Sampling Port Hole (in a vertical axis on the Stack Wall).

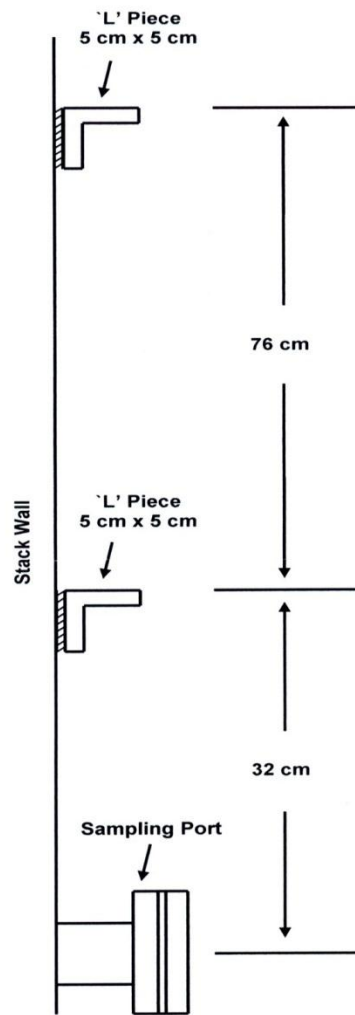

Fixing of 'L' Pieces on the Stack Wall

REFERENCES

1. Bio-medical Waste Management Rules, 2016.
2. CPCB Guidelines for CBWTFs (2003).
3. CPCB Guidelines for BMW Incinerators (2003).
4. 'Disposal of Bio-medical Waste generated during Universal Immunization Programme' issued by CPCB.
5. 'Guidelines for Environmentally Sound Management of Mercury Waste Generated from the Health Care Facilities' issued by CPCB.
6. Annual Report 2014 submitted to CPCB by the SPCBs/PCCs.
7. Stationary Source Emission Monitoring –Modifications to be made to the Sampling Platform and Sampling Port Hole issued by National Reference Trace Organics Laboratory (NRTOL), CPCB.

-- OO --



MEDICAL POLLUTION CONTROL COMMITTEE

AN ISO 14001:2015 CERTIFIED COMPANY

21, E - Block, Panki, Kanpur, PIN - 208020

Mob. : 9235659305, 7522822282

E-mail: help@mpccindia.in • Website: mpccindia.in



दिनांक: 24/06/2025

सेवा में,
क्षेत्रीय अधिकारी,
उत्तर प्रदेश प्रदूषण नियंत्रण बोर्ड,
बस्ती।

विषय: संस्था मेसर्स मेडिकल पाल्यूशन कण्ट्रोल कमेटी, खलीलाबाद, संतकबीरनगर द्वारा वार्षिक रिपोर्ट जनवरी 2024 से दिसम्बर 2024 तक प्रेषित किये जाने के सम्बन्ध में।

महोदय,

उपरोक्त विषयक अवगत हो कि संस्था मेसर्स मेडिकल पाल्यूशन कण्ट्रोल कमेटी, द्वारा डी-33, UPSIDC इंडस्ट्रियल एरिया, खलीलाबाद, जनपद - संतकबीरनगर में स्थापित/संचालित कॉमन बायो मेडिकल वेस्ट ट्रीटमेंट फैसिलिटी (CBWTF) की वार्षिक रिपोर्ट निर्धारित प्रारूप फार्म - IV पर आपको सादर प्रेषित की जा रही है।

अतः आपसे निवेदन है कि संस्था द्वारा प्रेषित वार्षिक रिपोर्ट का अवलोकन करने की कृपा करें।
सधन्यवाद।

भवदीय
Vinay Kumar Verma

(डॉ० विनय कुमार वर्मा)

MBBS, MAMS, FAGS, (USA)

सचिव

मेडिकल पाल्यूशन कण्ट्रोल कमेटी



संलग्नक - फार्म - IV वार्षिक रिपोर्ट।

सूचनार्थ एवं आवश्यक कार्यवाही हेतु प्रतिलिपि प्रेषित -

- मुख्य पर्यावरण अधिकारी, वृत्त-6, उत्तर प्रदेश प्रदूषण नियंत्रण बोर्ड, गोमती नगर, लखनऊ।

Vinay Kumar Verma

(डॉ० विनय कुमार वर्मा)

MBBS, MAMS, FAGS, (USA)

सचिव

मेडिकल पाल्यूशन कण्ट्रोल कमेटी



Clean India
Green India

Form – IV (See rule 13)
ANNUAL REPORT

[To be submitted to the prescribed authority on or before 30th June every year for the period from January to December of the preceding year, by the occupier of health care facility (HCF) or common bio-medical waste treatment facility (CBWTF)]

Sl. No.	Particular	
1	Particulars of the Occupier	
	(i) Name of the authorized person (occupier or : operator of facility)	: Dr. V.K. Verma
	(ii) Name of HCF or CBMWTF	: Medical Pollution Control Committee
	(iii) Address for Correspondence	: 21, E-Block, Panki, Kanpur
	(iv) Address of Facility	: D-33, UPSIDC, Industrial Area, Khalilabad, Sant Kabir Nagar
	(v) Tel. No, Fax. No	: 9839111510
	(vi) E-mail ID	: mpcckhalilabad@gmail.com
	(vii) URL of Website	: www.mpcckanpur.com
	(viii) GPS coordinates of HCF or CBMWTF	: CBWTF 26.774778, 83.090829
	(ix) Ownership of HCF or CBMWTF	: Private
	(x). Status of Authorization under the Bio-Medical Waste (Management and Handling) Rules	: Authorization No: 26563354 Dated -18/09/2024 Valid upto 31-12-2028
	(xi). Status of Consents under Water Act and Air Act	: Ref No. 211565/UPPCB/Basti(UPPCBRO)/CTO/both/ SANT KABIR NAGAR/2024 Dated-13/09/2024 valid upto 31-12-2028
2	Type of Health Care Facility	:
	(i) Bedded Hospital	: 585
	(ii) Non-bedded hospital	: 1280
	Clinical Laboratory or Research Institute or Veterinary Hospital or any other)	
	(iii) License number and its date of expiry	: Not Available
3	Details of CBMWTF	:
	(i) Number of health care facilities covered by CBMWTF	: 1865
	(ii) No. of Beds covered by CBMWTF	: 6202 beds (Bed in HCF 5658+1280 Non Bedded)
	(iii) Installed treatment and disposal capacity of CBMWTF :	: 6500 Kg Per Day
	(iv) Quantity of bio medical waste treated or disposed by CBMWTF	: 1095 Kg Per Day
4	Quantity of waste generated or disposed in Kg per Annum (on monthly average basis)	: Yellow Category : 652 Kg Per Day Red Category : 265 Kg Per Day White Category : 110 Grams Blue Category : 105 Kg Per Day General Solid Waste : 73 Kg/Day
5	Details of the Storage, Treatment, Transportation, Processing and Disposal Facility	
	(i) Details of the on-site storage facility	: Size : (12X14)X3

		Capacity : 30,000 Kg Approx			
		Provision of on-site storage (cold storage or any other provision) : Air cold storage room			
	(ii) Disposal facilities	Type of treatment equipment	No of Units	Capacity Kg/day	Quantity Treated or disposed in kg Per annum
		Incinerators	1	2400 Kg	237980 Kg
		Plasma Pyrolysis			
		Autoclaves	1	12000 Lit	96725 Kg
		Microwave			
		Hydroclave			
		Shredder	1	2400 Kg	NA
		Needle tip cutter or destroyer			
		Sharps Encapsulation or concrete pit	2		
		Deep burial pits	NA		
		Chemical disinfection:	1	800 Lit	38325 Kg
		Any other treatment equipment:			
	(iii) Quantity of recyclable wastes sold to authorized recyclers after treatment in Kg per annum	: Red Category (like plastic, glass, etc.) Handled by CBWTF Operator : 135050 Kg			
	(iv) No. of Vehicles used for collection and transportation of biomedical waste	20+1			
	(v) Details of incineration ash and ETP sludge generated and disposed during the treatment of wastes in Kg per annum	:		Quantity Generated	Where disposed
			Incineration Ash	4759 Kg	Bharat oil & waste Management Ltd., Kumbhi, Kanpur Dehat
			ETP Sludge	605 Kg	Incinerate by incinerator
	(vi) Name of the Common Bio- Medical Waste Treatment Facility Operator through which wastes are disposed of	Medical Pollution Control Committee			
	(vii) List of member HCF not handed over bio- medical waste.	N/A			
6	Do you have bio-medical waste management committee? If yes, attach minutes of the meetings held during the reporting period	N/A			

7	Details trainings conducted on BMW	
	(i) Number of trainings conducted on BMW Management	4 Training per annum
	(ii) Number of personnel trained	1580
	(iii) Number of personnel trained at the time of induction	118
	(iv) Number of personnel not undergone any training so far	N/A
	(v) Whether standard manual for training is available?	Yes
8.	Details of the accident occurred during the year	
	(i) Number of Accidents occurred	Nil
	(ii) Number of persons affected	Nil
	(iii) Remedial Action taken (Please attach details if any)	Nil
	(iv) Any Fatality occurred, details	Nil
	Are you meeting the standards of air Pollution from the incinerator? How many times in last year could not met the standards?	Every time meet the standards
	Details of Continuous online emission monitoring systems installed	Yes
	Liquid waste generated and treatment methods in place. How many times you have not met the standards in a year?	Every time meet the standards
	Is the disinfection method or sterilization meeting the log 4 standards? How many times you have not met the standards in a year?	Autoclaving and chemical disinfected all the time
	Any other relevant information	Air Pollution Control Devices attached with the incinerator

Certified that the above report is for the period from 1st January 2024 to 31st December 2024

(Dr. V.K. Verma)



Date: 24/06/2025

Place: Khalilabad

- TRUE COPY -



MEDICAL POLLUTION CONTROL COMMITTEE

AN ISO 14001:2015 CERTIFIED COMPANY

21, E - Block, Panki, Kanpur, PIN - 208020

Mob. : 9235659305, 7522822282

E-mail: help@mpccindia.in • Website: mpccindia.in



दिनांक: 04-06-2025

सेवा में,
सदस्य सचिव,
उत्तर प्रदेश प्रदूषण नियंत्रण बोर्ड,
गोमती नगर, लखनऊ

विषय: संस्था के विरुद्ध पर्यावरण (संरक्षण) अधिनियम 1986 यथासंशोधित की धारा-5 के अन्तर्गत जारी निर्देशों तथा नए HCFs के पंजीकरण की अनुमति के संबंध में।

महोदय,

सविनय निवेदन है कि वर्तमान में हमारी संस्था द्वारा महाराजगंज, कुशीनगर एवं सिद्धार्थ नगर जनपदों में बायो-मेडिकल वेस्ट के निस्तारण हेतु सेवाएं प्रदान की जा रही हैं। संस्था के विरुद्ध **Environment (Protection) Act, 1986 की धारा 5** के अंतर्गत निर्देश जारी किए गए थे, जिनके अंतर्गत वर्तमान में Medical Pollution Control Committee (MPCC) द्वारा कोई भी नया सदस्य पंजीकृत किए जाने पर रोक लगाई गई थी।

इस सम्बन्ध में आपको अवगत कराना है की उपरोक्त जनपदों में दो नई **Common Bio-Medical Waste Treatment Facility (CBWTF)** के संचालन में आने के कारण यह स्थिति उत्पन्न हुई है कि कई सरकारी एवं निजी स्वास्थ्य संस्थान अब हमारी सेवा क्षेत्र से बाहर जाकर अन्य CBWTF से जुड़ गए हैं। इन संस्थानों का विवरण निम्नवत है:

क्रम संख्या	स्वास्थ्य संस्थान (HCF) का नाम	जनपद	बेड्स की संख्या
1	सिद्धार्थ नगर CMO से सम्बद्ध शासकीय मेडिकल स्वस्थ संस्था	सिद्धार्थ नगर	462
2.	सिद्धार्थ नगर मेडिकल कॉलेज	सिद्धार्थ नगर	500
3.	KMC मेडिकल कॉलेज	महाराजगंज	500
4.	महाराजगंज CMO से सम्बद्ध शासकीय मेडिकल स्वस्थ संस्था	महाराजगंज	565
5.	कुशीनगर मेडिकल कॉलेज	कुशीनगर	500
6.	कुशीनगर CMO से सम्बद्ध शासकीय मेडिकल स्वस्थ संस्था	कुशीनगर	522
7.	AIIMS	गोरखपुर	750
8.	विभिन्न निजी HCFs (सूची सलग्न)	विभिन्न स्थानों	400
		कुल बेड्स	4199



Clean India
Green India

उपरोक्त परिस्थितियों के कारण हमारी संस्था की सेवा सीमा से कुल लगभग 4000 बेड्स बाहर हो गए हैं। पूर्व में उत्तर प्रदेश प्रदूषण नियंत्रण बोर्ड द्वारा निर्धारित 75 किमी परिधि में हमारी संस्था द्वारा 9000 बेड्स पर सेवाएं दी जा रही थीं, जो अब घटकर 5000 बेड्स तक सीमित रह गई हैं।

इस कारणवश, हमारी संस्था की उपचार क्षमता का समुचित उपयोग संभव नहीं हो पा रहा है। अतः निवेदन है कि परिस्थितियों में आए इस व्यावहारिक परिवर्तन को दृष्टिगत रखते हुए हमें नए हेल्थ केयर फैसिलिटीज (HCFs) के पंजीकरण की अनुमति प्रदान की जाए।

संस्था के विरुद्ध पर्यावरण (संरक्षण) अधिनियम 1986 यथासंशोधित की धारा-5 के अन्तर्गत निर्देश जारी किये गये गये जिनका अनुपालन संस्था द्वारा कर लिया गया है।

1. शिकायती स्थल ग्राम बनकटवा, पोस्ट बेलैली, जनपद-संतकबीरनगर पर डंप किये गए जैव चिकित्सा अपशिष्ट को संस्था द्वारा सुरक्षित निस्तारित एवं डंप स्थल पर Remediation Work भी पूर्ण करवा दिया गया है।

अतः आपसे विनम्र अनुरोध है कि कृपया संस्था के विरुद्ध पर्यावरण (संरक्षण) अधिनियम 1986 यथासंशोधित की धारा-5 के अन्तर्गत जारी निर्देश को निरस्त (Remove/Withdraw) करने की कृपा करें, एवं संस्था को नए HCFs के पंजीकरण की अनुमति प्रदान करने की कृपा करें, ताकि हमारी बची हुई उपचार क्षमता का उपयोग क्षेत्र में सुरक्षित एवं नियंत्रित बायो-मेडिकल वेस्ट प्रबंधन हेतु किया जा सके।

सधन्यवाद।

भवदीय



(डॉ० विनय कुमार वर्मा)

MBBS, MAMS, FAGS (USA)

सचिव,

मेडिकल पाल्यूशन कण्ट्रोल कमेटी

संलग्नक - बंद एवं अन्य संस्था (CBWTF) के साथ पंजीकृत HCFs की सूची

निम्न को सूचनार्थ एवं आवश्यक कारवाही हेतु प्रतिलिपि प्रस्तुत

1. मुख्या पर्यावरण अधिकारी, वृत्त 6, उत्तर प्रदेश प्रदूषण नियंत्रक बोर्ड, लखनऊ
2. क्षेत्रीय अधिकारी, उत्तर प्रदेश प्रदूषण नियंत्रक बोर्ड, बस्ती

डाक प्राप्ति रसीद

प्राप्ति दिनांक.....

प्राप्तकर्ता के हस्ताक्षर.....

उ०प्र० प्रदूषण नियंत्रक बोर्ड, लखनऊ

04/06/25




(डॉ० विनय कुमार वर्मा)

MBBS, MAMS, FAGS (USA)

सचिव,

मेडिकल पाल्यूशन कण्ट्रोल कमेटी

Guidelines for Common Bio-medical Waste Treatment and Disposal Facilities



CENTRAL POLLUTION CONTROL BOARD

(Ministry of Environment, Forest and Climate Change)

Parivesh Bhawan, East Arjun Nagar

DELHI - 110 032

website: www.cpcb.nic.in

(April 12, 2025)

Abbreviations

APCD	-	Air Pollution Control Device
BMWM Rules	-	Bio-medical Waste Management Rules, 2016
CBWTF	-	Common Bio-medical Waste Treatment and Disposal Facility
CO	-	Carbon Monoxide
CO ₂	-	Carbon Dioxide
CPCB	-	Central Pollution Control Board
CRZ	-	Coastal Regulation Zone
DG	-	Diesel Generator
EC	-	Environmental Clearance
EIA	-	Environment Impact Assessment
ETP	-	Effluent Treatment Plant
GPS	-	Global Positioning System
HCFs	-	Health Care Facilities
HCl	-	Hydrochloric Acid
HOWM & TM Rules	-	Hazardous and Other Waste (Management & Transboundary Movement) Rules, 2016
MHz	-	Mega Hertz
MoEF& CC	-	Ministry of Environment, Forest & Climate Change
KM	-	Kilometer
KW	-	Kilowatt
MoU	-	Memorandum of Understanding
NABL	-	National Accreditation Board for Testing and Laboratories
NO _x	-	Oxides of Nitrogen
O ₂	-	Oxygen
PCC	-	Pollution Control Committee
PLC	-	Programmable Logical Control
SEIAA	-	State Environment Impact Assessment Authority
SLF	-	Secured Landfill
SPCB	-	State Pollution Control Board
TSDF	-	Treatment Storage and Disposal Facility
TOC	-	Total Organic Carbon
VOCs	-	Volatile Organic Compounds

CONTENT

S. No	Description	Page No.
1	Introduction	01
2	Criteria for development of a new Common Bio-medical Waste Treatment and Disposal Facility	02
3	Duties of the operator of a common bio-medical waste treatment and disposal facility	06
4	Applicability of the guidelines	06
5	Environmental laws applicable for commissioning or operation of a CBWTF	07
6	Location criteria	08
7	Land requirement	09
8	Coverage area of CBWTF	10
9	Treatment equipment	10
10	Infrastructure set up	16
11	Record keeping	21
12	Collection and transportation of bio-medical waste	25
13	Disposal option of solid waste generated from CBWTF	29
14	Cost to be charged by the CBWTF operator for the Health Care Facilities	30
15	Check list for development of CBWTF	31
16	Periodic inspection/monitoring or performance evaluation of the CBWTFs	31
	List of Figure and Table	
	Figure 1. Criteria for development of a CBWTF in a coverage area	05
	Table 1: Suggested validation test for treatment of bio-medical waste by autoclave/microwave/chemical treatment/dry heat sterilization	24
	Table 2: Suggested disposal option of solid waste generated from CBWTF	29
	List of Annexure	
	Annexure-I: Coverage area-wise gap analysis for assessing additional BMW treatment capacity requirement	35
	Annexure -II: Format for maintaining the record by the CBWTF Operator along with the transportation vehicle used for collection of the Bio-medical waste from the member HCFs	36
	Annexure -III: Log Book for operating the Incinerator/Plasma Pyrolysis and Autoclave	37
	Annexure -IV: Check list for Development of a CBWTF	38
	Annexure -V: Check list for Performance Evaluation of the CBWTF	43
	Annexure -VI: Stationary Source Emission Monitoring for Dioxins and Furans	56
	Annexure -VII: Details regarding colour and size of bio-hazard symbol and font	59

	List of Appendix	
	Appendix I: Methodology to conduct gap analysis with respect to generation and treatment of biomedical waste- Rev.1	32
	References	61

1) Introduction

A Common Bio-medical Waste Treatment and Disposal Facility (CBWTF) is a set up where biomedical waste generated from member health care facilities is imparted necessary treatment to reduce adverse effects that this waste may pose on human health and environment. The treated recyclable waste may finally be sent for disposal in a secured landfill or for recycling.

According to the Bio-medical Waste Management Rules, 2016, "bio-medical waste treatment and disposal facility" means any facility wherein treatment, disposal of bio-medical waste or processes incidental to such treatment and disposal is carried out, and includes common bio-medical waste treatment facilities and "operator of a common bio-medical waste treatment facility" means a person who owns or controls a Common Bio-medical Waste Treatment and Disposal Facility (CBWTF) for the collection, reception, storage, transport, treatment, disposal or any other form of handling of bio-medical waste.

The Bio-medical Waste Management Rules, 2016 (BMWM Rules) restricts occupier for establishment of on-site or captive bio-medical waste treatment and disposal facility, if a service of common bio- medical waste treatment and disposal facility is available within a distance of seventy-five kilometer, as installation of individual treatment facility by health care facility (HCF) requires comparatively high capital investment. In addition, it requires separate dedicated and trained skilled manpower and infrastructure development for proper operation and maintenance of treatment systems. The concept of CBWTF not only addresses such problems but also prevents proliferation of captive treatment facilities in a particular area. In turn, it reduces the monitoring pressure on regulatory agencies. By running the treatment equipment at CBWTF to its full capacity, the cost of treatment of per kilogram of bio-medical waste gets significantly reduced. Its considerable advantages have made CBWTF popular and proven concept in most part of the world.

The CBWTFs are also required to set up based on the need for ensuring environmentally sound management of bio-medical waste keeping in view the techno-economic feasibility and viable operation of the facility with minimal impact on human health and environment.

Since 1998, the CBWTF as an option for treatment of bio-medical waste also been legally introduced in India. Considering the likely impacts that may cause to the

patients undergoing treatment because of operation of the captive treatment equipment within the health care facilities (HCFs), now the Bio-medical Waste Management Rules, 2016 recommends the Occupier (i.e., HCF) for ensuring treatment and disposal of generated bio-medical waste through a CBWTF, located within a distance of 75 KM. Further, these rules eased the bottleneck in upbrining the CBWTF by making department in the business allocation of land assignment in the State or UT administration responsible for providing a suitable site (s) within its jurisdiction.

The concept of CBWTF is also being widely accepted in India among the healthcare units, medical associations and entrepreneurs. In order to set up a CBWTF to its maximum perfection, care shall be taken in choosing the right technology, development of CBWTF area, proper designing of transportation system to achieve optimum results etc. Key features of CBWTF have been addressed in the subsequent sections.

To facilitate the treatment and disposal of bio-medical waste generated from the HCFs, at present (as per Annual Report 2023 submitted by the State Pollution Control Boards/Pollution Control Committees), there are 234 no. of CBWTFs in operation and 30 no. of CBWTFs are under construction. Also, the Bio-medical Waste Management Rules, 2016 mandates that the operator of a CBWTF authorised by the prescribed authority is required to take all necessary steps to ensure that the bio-medical waste collected from the occupier is transported, handled, stored, treated and disposed of, without any adverse effect to the human health and the environment, in accordance with the BMW Rules and the guidelines issued by the Central Government or the Central Pollution Control Board (CPCB) from time to time. Therefore, these guidelines have been prepared with an aim to have uniformity in ensuring site selection, allowing and establishment of a state-of-the-art CBWTF, operation as well as verification of compliance to the BMW Rules, 2016 throughout the country. However, any other aspects which are not been covered under these guidelines and needs attention, in such a case, the prescribed authority may take suitable action in the interest of protection of the environment in consultation with MoEF & CC/CPCB. Also, it is pertinent to mention here that these guidelines are mandatory henceforth under the Bio-medical Waste Management Rules, 2016

2) Criteria for development of a new Common Bio-medical Waste Treatment and Disposal Facility for a locality or region.

Prior to allowing any new CBWTF, following criteria or steps may be followed:

-
- a) Prescribed authority under the BMWM Rules, 2016 [i.e., State Pollution Control Board (SPCB) in the respective State or Pollution Control Committee (PCC) in the respective Union Territory Administration] is required to prepare an inventory or review with regard to the bio-medical waste generation at least once in five years in the coverage areas of the existing bio-medical waste treatment and disposal facility. The prescribed authority is also required to extrapolate the coverage-area wise bio-medical waste generation for the next ten years.
 - b) SPCB/PCC is required to conduct gap analysis w.r.to coverage area of the bio-medical waste generation, its projection over a period of next ten years, adequacy of existing treatment capacity of the CBWTF in each coverage area of radius 75 KM, as given in **Annexure-I** and as per methodology for conduct of gap analysis given at **Appendix-I**.

Further, decision may be taken by concerned SPCB/PCC based on gap analysis report to allow new facility or expansion of an existing facility. Adequacy of the existing facility to handle quantum of biomedical waste and/or compliance with the norms prescribed under BMWM Rules, 2016 shall also be taken into account.

All the SPCBs and PCCs shall conduct the gap analysis and based on the gap analysis, action plan for development of new CBWTFs is required to be prepared and submitted to MoEF & CC & CPCB within six months' time. In case of States/UTs, where no CBWTF is available, in such a case, SPCB/PCC being prescribed authority under the BMWM Rules is required to ensure establishment new facilities. SPCB/PCC may submit the detailed proposal to MoEF & CC/MoH & FW through the respective State Government or UT Administration. Association of HCFs may also be encouraged to develop their own CBWTF following these guidelines. In case, any coverage area requires additional treatment capacity, in such a case, action may be initiated by the prescribed authority for allowing a new CBWTF in that locality based on the gap analysis report without interfering the coverage area of the existing CBWTF.

- c) SPCB/PCC shall identify the coverage area, which require additional treatment facility and bring it to the notice of the concerned department in the business allocation of land assignment in the respective State Government or UT Administration. The department in the business allocation of land assignment shall be responsible for providing suitable site in the identified coverage area for setting up of a CBWTF, in
-

consultation with the prescribed authority (i.e., SPCB/PCC), other stakeholders and in accordance with these guidelines issued by CPCB from time to time.

- d) Alternately, a CBWTF may also be allowed to be established on a land procured by an entrepreneur in accordance with the location criteria suggested under these guidelines.
- e) The SPCB/PCC or concerned department in the business allocation of land assignment in the respective State Government or UT Administration may seek expression of interest from the proponents for development of new CBWTF (s) in the identified coverage area. Upon allocation of site to the proponent, the proponent is required to take necessary approvals as required under the Environment (Protection) Act, 1986 for development of the new CBWTF in accordance with these guidelines.
- f) In the absence of expression of interest by any proponent, then SPCB/PCC shall insist health care facilities to form association and to develop its own CBWTF in line with these guidelines or to have captive treatment facilities (Only hilly or remote areas) for ensuring treatment and disposal of generated bio-medical waste as stipulated under the BMWM Rules.
- g) In case of any regulatory action including closure of any existing CBWTF is inevitable, the respective SPCB/PCC may take action under the BMWM Rules including for making alternate arrangement to ensure safe disposal of the bio-medical waste generated from the member health care facilities of such default CBWTF through CBWTF located nearby.
- h) In case of hilly areas considering the geography, only one CBWTF with adequate treatment capacity may be developed covering at least two districts to cater treatment services to the HCFs located in the respective Districts. The selection and allocation of site etc., should be done as per the criteria suggested under these guidelines. The treatment charges to be prescribed by the respective SPCB/PCC in consultation with the State Advisory Committee.

The criteria for development of CBWTFs in any coverage area is also depicted in **Figure 1**.

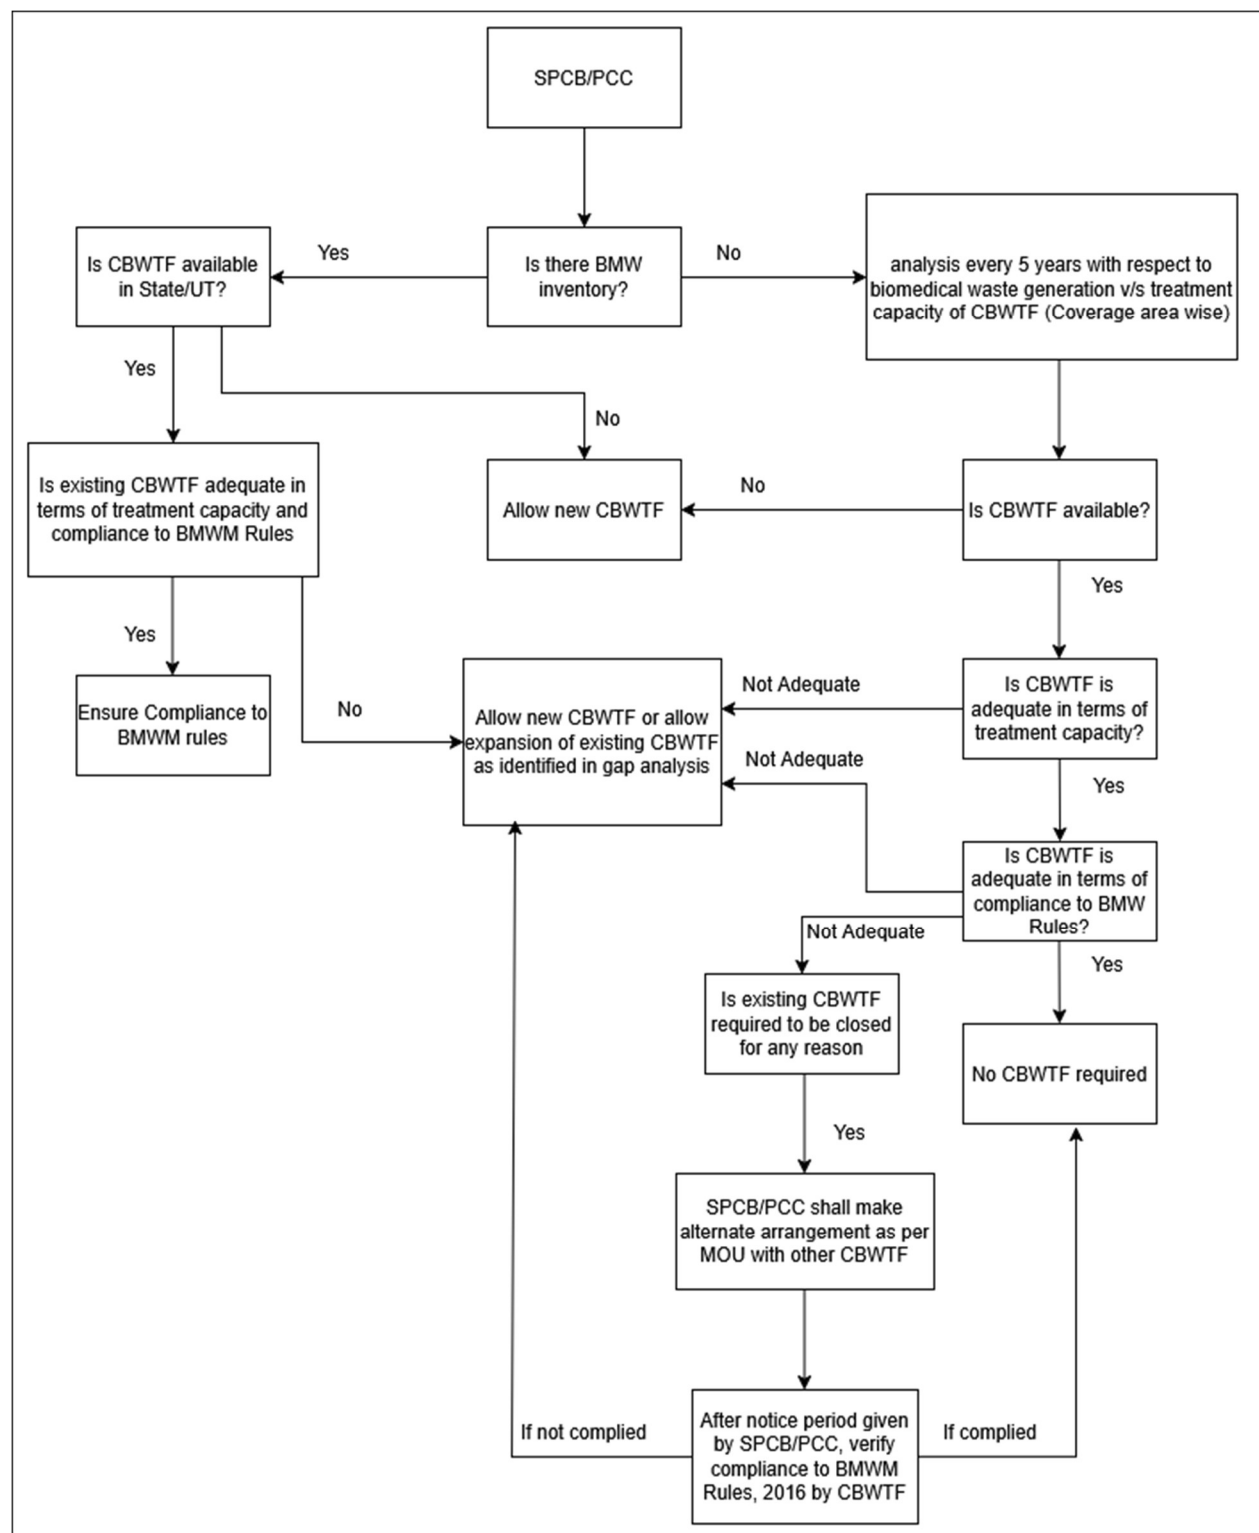


Figure 1. Criteria for Development of a CBWTF in a coverage area

3) **Duties of the operator of a common bio-medical waste treatment and disposal facility**

The duties of the operator of a common bio-medical waste treatment and disposal facility (CBWTF) as enunciated under Rule 5 of the Bio-medical Waste Management Rules, 2016 shall be ensured and complied with. All CBWTFs shall also comply w.r.to the residence time as well as emission norms including for Dioxins and Furans for incineration facility as prescribed under BMWM Rules, 2016. In addition to the above, to ensure proper management of bio-medical waste in the respective coverage area, as a mitigation measure, especially in the event of

- (a) a temporary break down (not more than a week) of a CBWTF especially for rectification of the refractory lining of the incineration chambers or change of requisite APCD due to failure; and
- (b) Closure of a CBWTF for violation of the provisions of the BMWM Rules or any other reason.

All CBWTFs are required to submit action plan (in case of closure), to the respective SPCB/PCC, for imposing suitable condition while granting authorisation under the BMWM Rules, 2016. The action plan should include:

- (a) an MoU made with the nearest two CBWTF located within the respective State/UT as alternate arrangement ensuring that the bio-medical waste generated is collected, treated and disposed of within 48 hours as stipulated under the BMWM Rules. In case, if there is no CBWTF located nearby then such CBWTF should have to install stand by treatment equipment (equal to the existing treatment capacity as per consents granted by the SPCB/PCC), and
- (a) Decontamination plan of the CBWTF for execution of such plan prior to closure of a CBWTF.

4) **Applicability of these guidelines**

These guidelines are applicable to all the upcoming or new CBWTFs. In case of the existing CBWTFs, these guidelines shall be applicable

- (a) the existing CBWTFs desires to expand or enhance the existing treatment capacity
(or)
 - (b) the existing CBWTFs desires to modernize the existing treatment equipment with the new equipment with enhancement in the existing treatment capacity.
-

5) Environmental laws applicable for commissioning or operation of a CBWTF

Operation of a CBWTF leads to air emissions as well as waste water generation as in case of an industrial operation. Most common sources of waste water generation in CBWTFs are vehicle washing, floor washing, and scrubbed liquid effluent from air pollution control systems attached with the incinerator/plasma pyrolysis. Incineration as well as DG Set is the general source of air emissions.

5.1 Any other approvals (such as Land Use /Change in Land Use as applicable) required from the concerned authorities under various laws have to be complied with by the proponent of the CBWTF prior to development of a CBWTF.

5.2 Consents under Water (Prevention and Control of Pollution) Act, 1974 and Air (Prevention and Control of Pollution) Act, 1981 as well as Authorization under the BMWM Rules, 2016

The project proponent of the CBWTF is required to obtain 'Consent to Establishment' under Section 25 of the Water (Prevention and Control of Pollution) Act, 1974 and Section 21 of the Air (Prevention and Control of Pollution) Act, 1981, from the respective prescribed authority i.e. SPCB/PCC. Upon installation of the requisite equipment, the CBWTF Operator is also required to obtain authorization under BMWM Rules, 2016 co-terminus with consent to operate under Water (Prevention and Control of Pollution) Act, 1976 & Air (Prevention and Control of Pollution) Act, 1981 from the respective SPCB/PCC prior to commencement of the CBWTF.

5.3 Environmental Clearance under EIA Notification 2006

Ministry of Environment, Forest & Climate Change (MoEF & CC), notified amendment to the EIA Notification 2006 and published vide MoEF & CC Notification of S.O. 1142 (E) dated April 17, 2015. According to this notification, the 'bio-medical waste treatment facility' is categorized under the Item 7 (da) in the schedule, requiring 'environmental clearance' from the State Environment Impact Assessment Authority (SEIAA). Therefore, the CBWTF operator is also required to obtain 'Environmental Clearance (EC)' from the respective SEIAA or Ministry of Environment, Forest & Climate Change (MoEF & CC), as the case may be, before any construction work, or preparation of land by the projects management, which include the following:

a) All new projects or activities pertaining to the bio-medical waste treatment facility; and

- b) Expansion and modernization with additional treatment capacity of existing bio-medical waste treatment facility (excluding augmentation of incineration facility for compliance to the residence time as well as Dioxins and Furans without enhancing the existing treatment capacity).
- c) Any expansion or modification in the treatment capacity or relocation of the existing CBWTF (requires compliance to the relevant provisions notified under the Environment (Protection) Act, 1986 by the MoEF & CC.

6) Location criteria

In the context of these guidelines, buffer zone represents a separation distance between the source of pollution in CBWTF and the receptor - following the principle that the degree of impact reduces with increased distance. The following parameters may be considered for ascertaining buffer distance on case-to-case basis:

- (i) potential for spread of infection from wastes stored in the premises.
- (ii) applicable standards for pollution control and the relative efficiency of the existing incinerators and emission control systems,
- (iii) potential of fugitive dust emission from incinerators,
- (iv) Quantity and quality of wastewater discharged
- (v) the potential for odour production,
- (vi) the potential for noise pollution,
- (vii) the risk posed to human health due to exposure to emissions from incinerator,
- (viii) the risk of fire and
- (ix) significance of the residual impacts such as bottom ash and fly ash.

As far as possible, the CBWTF shall be located near to its area of operation in order to minimize the transportation distance in waste collection, thus enhancing its operational flexibility as well as for ensuring compliance to the time limit for treatment and disposal of bio-medical waste as stipulated under the BMW Rules (i.e., within 48 hours). Also, the location of the CBWTF should be in conformity to the CRZ Norms and other provisions notified under the Environment (Protection) Act, 1986. The location shall be decided in consultation with the State Pollution Control Board (SPCB)/ Pollution Control Committee (PCC) and SEIAA or MoEF & CC, as the case may be. The location criteria for development of a CBWTF are as follows:

- (a) A CBWTF shall preferably be developed in a notified industrial area without any requirement of buffer zone **(or)**

-
- (b) A CBWTF can be located at a place reasonably far away from notified residential and sensitive areas and should have a buffer distance of preferably 500 m so that it shall have minimal impact on these areas. In case of non-availability of such a land, the buffer zone distance from the notified residential area may be reduced to less than 500 m by SPCB/PCC without referring the matter to CPCB by prescribing additional control measures such as (i) adoption of best available technologies (BAT) by the proponent of CBWTF; (ii) prescribing stringent standards for operation of the CBWTF by the SPCB/PCC; (iii) adoption of zero liquid discharge by the CBWTF and (iv) in case of any complaints from the public, then CBWTF should prove that the facility is not causing any adverse impact on environment and habitation in the vicinity.
 - (c) The CBWTF can also be developed as an integral part of the Hazardous Waste Treatment Storage and Disposal Facility (TSDF) subject to obtaining of necessary approvals from the authorities concerned including 'environmental clearance' as per Environmental Impact Assessment 2006 and further amendments notified under the Environment (Protection) Act, 1986, provided there is no CBWTF exist within 150 KM distance from the existing TSDF.

7) Land requirement

Sufficient land shall be allocated to the CBWTF to provide all requisite systems which include dedicated space for storage of waste (both treated and untreated), waste treatment equipment, vehicle washing bay, vehicle parking space, ETP, incineration ash storage provision, administrative room, space for DG Set etc.,.

- (a) Preferably, a CBWTF shall be set up on a plot size of not less than one acre in all the areas. However, a CBWTF can be developed in adjacent plots but cannot be set up in two or more different plots located in different areas. Separate plots can be permitted only for vehicle parking if located in the close vicinity of the proposed CBWTFs or the existing CBWTFs.
 - (b) In case of upcoming or new CBWTFs (where municipal population is more than 25 lakhs), the land area requirement may be relaxed (but in any case not less than 0.5 acre) by the SPCB/PCC, with additional control measures such as zero liquid discharge, increase in stack height, stringent emission norms, odour control measures or any other measures felt necessary by the prescribed authority on case-to-case basis, only in consultation with SEIAA or MoEF &CC, as the case may be.
-

8) Coverage area of CBWTF

Suggested coverage area for development of a CBWTF is as follows:

- a) A CBWTF located within the respective State/Union Territory may be allowed to cater to healthcare units situated within a radial distance of 75 kilometers, subject to the condition that the facility possesses adequate treatment capacity to handle the bio-medical waste generated within the said radius. For the purpose of determining adequacy, 90% of the total treatment capacity as authorized by the concerned State Pollution Control Board (SPCB) or Pollution Control Committee (PCC) shall be considered. It shall further be ensured that bio-medical waste generated is collected, treated and disposed of within 48 hours as stipulated under the BMWM Rules.

The concerned SPCB/PCC shall undertake a gap analysis, as per **Appendix-I**, to assess the quantum of bio-medical waste generated vis-à-vis the available treatment capacity of the CBWTF (considering 90% of the authorized treatment capacity). In case the analysis indicates a shortfall in treatment capacity or if the existing CBWTF is found to be non-compliant with the provisions of the Bio-Medical Waste Management Rules, 2016, the SPCB/PCC may consider proposals for establishing a new CBWTF or for expansion of an existing facility, ensuring that bio-medical waste generated is collected, treated and disposed of within 48 hours as stipulated under the BMWM Rules.

- b) In case of hilly areas, considering the geography, only one CBWTF with adequate treatment capacity may be developed covering at least two districts to cater treatment services to the HCFs located in the respective Districts. The selection and allocation of site etc. should be done as per the criteria suggested under these guidelines. The treatment charges to be prescribed by the respective SPCB/PCC in consultation with the State Advisory Committee to be constituted under the BMWM Rules by the respective State Government or UT Administration.

9) Treatment equipment

The Common Bio-medical Waste Treatment Facility should treat the bio-medical waste as per BMWM Rules and as per the authorisation granted by the prescribed authority. The CBWTF should have the following treatment facilities:

a) Incineration/Plasma Pyrolysis

Incineration is a controlled combustion process where waste is completely oxidized and harmful microorganisms present in it are destroyed/ denatured under high temperature. The guidelines for "Design & Construction Requirements of Bio-medical Waste Incinerators" by CPCB from time to time shall be followed for selecting/or augmenting the incinerator.

Plasma Pyrolysis is an alternate to incinerator, Plasma Pyrolysis treatment technology can be installed for disposal of bio-medical waste categories as per BMWWM Rules wherein destruction of bio-medical waste is similar to incineration can be achieved. In case of plasma pyrolysis, waste is treated at high temperature under controlled condition to form gases like methane, hydrogen and carbon monoxide which are subjected to combustion (oxidation) in secondary chamber. In the plasma pyrolysis process waste is converted into small clinker which can be disposed in secured landfills.

b) Autoclaving/Hydroclaving/Microwaving

- (i) **Autoclaving** is a low-heat thermal process where steam is brought into direct contact with waste in a controlled manner and for sufficient duration to disinfect the wastes as stipulated under the Bio-medical Waste Management Rules. For ease and safety in operation, the system should be horizontal type and exclusively designed for treatment of bio-medical waste. For optimum results, pre-vacuum based system be preferred against the gravity type system. It shall have tamper-proof control panel with efficient display and recording devices for recording critical parameters such as time, temperature, pressure, date and batch number etc. as required under the BMWWM Rules.
 - (ii) **Hydroclaving** is similar to that of autoclaving except that the waste is subjected to indirect heating by applying steam in the outer jacket. The waste is continuously tumbled in the chamber during the process.
 - (iii) **Microwaving:** In microwaving, microbial inactivation occurs as a result of the thermal effect of electromagnetic radiation spectrum lying between the frequencies 300 and 300,000MHz. Microwave heating is an inter-molecular heating process. The heating occurs inside the waste material in the presence of steam.
-

-
- c) Chemical disinfection:** Though chemical disinfection or alternates as stipulated under the BMWM Rules is also an option for treatment of certain categories of bio-medical waste such as glass waste but looking at the volume of waste to be disinfected at the CBWTF and the pollution load associated with the use of chemical disinfectants, the chemical disinfection for treatment of bio-medical waste as part of a CBWTF may be used sparingly or avoided as far as possible.
- d) Dry heat sterilization:** This is the additional option for treatment of waste sharps as stipulated under the BMWM Rules. In this method, waste sharps are treated using dry heat (hot air) at a temperature not less than 185°C, at least for a residence period of 150 minutes in each cycle (with sterilization period of 90 minutes).
- e) Shredder:** Shredding is a process by which waste are de-shaped or cut into smaller pieces so as to make the wastes unrecognizable. It helps in prevention of reuse of bio-medical waste and also acts as identifier that the wastes have been disinfected and are safe to dispose of. A shredder to be used for shredding bio-medical waste shall confirm to the following minimum requirements:
- (i) The shredder for bio-medical waste shall be of robust design with minimum maintenance requirement;
 - (ii) The shredder should be properly designed and covered to avoid spillage and dust generation. It should be designed such that it has minimum manual handling;
 - (iii) The hopper and cutting chamber of the shredder should be so designed to accommodate the waste bag full of bio-medical waste;
 - (iv) The shredder blade should be highly resistant and should be able to shred waste sharps, syringes, scalpels, blades, plastics, catheters, intravenous sets/ bottles, blood bags, gloves, bandages etc. It should be able to handle/ shred wet waste, especially after microwave/ autoclave/hydroclave;
 - (v) The shredder blade shall be of non-corrosive and hardened steel;
 - (vi) The shredder should be so designed and mounted so as not to generate dust, high noise & vibration;
 - (vii) If hopper lid or door of collection box is opened, the shredder should stop automatically for safety of operator;
 - (viii) In case of shock-loading (non-shreddable material in the hopper), there should be a mechanism to automatically stop the shredder to avoid any emergency/accident;
-

-
- (ix) In case of overload or jamming, the shredder should have mechanism of reverse motion of shaft to avoid any emergency/accident;
 - (x) The motor shall be connected to the shredder shaft through a gear mechanism, to ensure low rpm and safety;
 - (xi) The unit shall be suitably designed for operator safety, mechanical as well as electrical;
 - (xii) The shredder should have low rotational speed (maximum 50 rpm). This will ensure better gripping and cutting of the bio-medical waste;
 - (xiii) The discharge height (from discharge point to ground level) shall be sufficient (minimum 3 feet) to accommodate the containers for collection of shredded material. This would avoid spillage of shredded material;
 - (xiv) The minimum capacity of the motor attached with the shredder shall be 3 KW for 50 Kg/hr, 5 KW for 100 kg/hr & 7.5 KW for 200 Kg/hr and shall be three phase induction motor. This will ensure efficient cutting of the bio-medical wastes as prescribed in the Bio-medical Waste Management Rules; and
 - (xv) The shredder also should be fitted with separate 'energy meter' for recording total energy consumed for operation of this equipment.

g) *Sharp pit/ Encapsulation:* A sharp pit or a facility for sharp encapsulation in a metal container or cement concrete shall be provided for treated sharps (*i.e., treatment by autoclaving or dry heat sterilization followed by shredding or mutilation*). An option may also be worked out for recovery of metal from treated and shredded waste sharps within the CBWTF or iron foundries having consent to operate from the SPCBs/PCCs and located nearby, as per the conditions imposed in authorization granted under BMW Rules by the SPCB/PCC.

A sharp pit may be of circular or rectangular shape and shall be dug and lined with cement plastered brick masonry or concrete rings. The pit should be covered with a heavy concrete slab with a provision of galvanized steel pipe projecting about 1.5 meters above the slab, with an internal diameter of up to 50 mm or 1.5 times the length of vials, whichever is more. The top opening of the steel pipe shall have a provision of locking after the treated waste sharps are disposed into the sharp pit. When the pit is full, it can be sealed completely, after another pit is prepared. In case of high water table regions (*i.e., where water table is less than 6 metres beneath the bottom of the sharp pit*), a tank with above mentioned arrangements shall be made above the ground.

-
- h) Deep burial:** SPCB/PCC should not allow the 'deep burial' of bio-medical waste as a part of CBWTF.
- i) Non-burn technology:** Non-incineration technologies for disposal of bio-medical waste are adopted in some of the developed countries. Non-incineration technology comprises of shredding and disinfection by autoclaving/microwaving or chemical treatment. The treated waste can be disposed along with municipal solid waste in sanitary landfills or through waste to energy plants. Such option can also be adopted in places where the sanitary landfill or waste to energy plant for disposal of municipal solid waste is available. Such technology is permitted only after prior approval of MoEF & CC and only after obtaining authorization under the BMWM Rules from the respective SPCB/PCC for the purpose of carrying out trial runs for assessment of efficacy of the treatment equipment.
- j) Vehicle/Containers washing facility:** Every time a vehicle is unloaded, the vehicle and empty waste containers shall be washed properly and disinfected. Washing can be carried out in an open area but on an impermeable surface and liquid effluent so generated shall be conveyed and treated in an effluent treatment plant. The impermeable area shall be of appropriate size so as to avoid spillage of liquid during washing.
- k) Effluent Treatment Plant:** A suitable Effluent Treatment Plant (ETP) shall be installed to ensure that liquid effluent generated during the process of washing containers, vehicles, floors etc. is treated and reused after treatment. Proper treatment of waste water shall be ensured in case of zero discharge by recirculation of treated waste water for scrubbing. ETP may have treatment unit operations comprising collection tank, O & G trap, chemical dosing cum mixing (Flash and slow), coagulation chamber, primary settling tank (s), biological treatment process, secondary settling tank, pressure filter and activated carbon filter, pH Correction tank (wherever recirculation of treated water is practiced) so as to comply with the liquid discharge standards stipulated under the Bio-medical Waste Management Rules, 2016. ETP may also have the following provisions:
- (i) separate 'energy meter' so as to know total consumption of electricity for operation of the machinery attached with the ETP.
-

- (ii) pH meter so as to know pH level of treated water as well as pH level of treated water used for recirculated or recycling in APCD attached with the incinerator or any utility within the CBWTF.
- (iii) A 'magnetic flow meter' should also be fitted at all the water supply extraction points of the CBWTF as well as the outlet to know the total wastewater treated for further end use or discharge in compliance to the BMWM Rules.
- (iv) Provision of 'press filter' to reduce the moisture content of the ETP Sludge or it may be dried in 'sludge drying bed'. After removal of moisture content or drying, same need to be disposed of in an environmentally sound manner depending upon the hazardous constituents present in it as per Hazardous and Other Waste (Management and Transboundary Movement) Rules, 2016. In case, ETP sludge contains metal contents within the prescribed limits as per Hazardous & Other Waste (Management & Transboundary Movement) Rules, 2016, such ETP sludge shall be given to CBWTF for incineration or to hazardous waste treatment, storage and disposal facility (TSDF) for disposal in secured landfill.

Note:

- a) If any CBWTF desires to adopt any other technology other than referred under Schedule –I of the BMWM Rules, may adopt new technology only with the prior approval from MoEF & CC and is also required to obtain authorization under the BMWM Rules from the respective SPCB/PCC for carrying out trial run for assessment of efficacy of the new technology.
- b) All the treatment equipment should be operated and complied with the norms as stipulated under Schedule II of the Bio-medical Waste Management Rules, 2016 published by MoEF & CC vide GSR 343 (E) dated 28th March, 2016.
- c) Incinerator / Plasma Pyrolysis/ Autoclaving/Microwaving/ Hydroclaving/ Shredder/ Dry Heat Sterilization/ ETP should be fitted with separate 'energy meter' for recording total energy consumed for operation of these equipment.
- d) In the event of temporary shutdown (not more than a week) due to any operational problems in the treatment equipment (such as restoration of refractory lining or maintenance or repairs in APCD), to ensure bio-medical waste collected from the member health care facilities is treated within the time limit as stipulated under the BMWM Rules, all CBWTF operators should also be provided with stand by treatment equipment especially incinerator/plasma pyrolysis/autoclave (or) alternately MoU made with the nearby CBWTF (located within the State/UT) shall be submitted to the respective SPCB/PCC, by all the existing CBWTF operators (whereas the upcoming facilities have to make such arrangement prior to commencement of the facility) so as to include such condition while granting authorisation under the BMWM Rules, 2016 to the concerned CBWTF operators (vice-versa).

(10) Infrastructure set up

The CBWTF shall have enough space within it to install required treatment equipment, untreated and treated waste storage area, vehicle-parking, vehicle and containers washing area, Effluent Treatment Plant (ETP), administration room or staff room etc. The required area for CBWTF would depend upon the projected amount of bio-medical waste to be handled by it. A CBWTF shall have the following infrastructure:

a) Treatment equipment room

A separate housing may be provided for each treatment equipment at the CBWTF such as incinerator room, autoclave room, microwave room etc., as applicable. Each room shall have well-designed roof and walls. Such room shall be well ventilated and easy to wash. The floor and interior finishing of the room shall be such that chances of sticking/harboring of microorganisms are minimized. This can be attained by providing smooth & fine floor and wall surfaces (to a height of 2 meter from floor) preferably of tiles. The number of joints in such surfaces shall be minimal. The equipment room shall also have a separate cabin, to supervise the operation of the equipment and to record the waste handling and equipment operational data attached to each equipment room. There shall be two waste storage rooms, one for storage of untreated waste and another for treated waste and may be located at a distance from each other. The storage room shall have provisions similar to that of equipment room being well-ventilated with easy to wash floors & walls, smooth and fine surfaces etc. All the treatment equipment rooms and waste storage rooms should be provided with 'fly catcher/killing device'. The room shall be washed and cleaned with a suitable disinfectant every day.

b) Main waste storage space

Separate space shall be provided near the entry point of the CBWTF to unload and store all biomedical wastes that have been transported to the CBWTF by its own transportation vehicle. The size of the room shall be adequate to store all wastes transported to the CBWTF. The front portion of the room shall be utilized for unloading the wastes from the vehicle and back or side portion shall be utilized for shifting the wastes to the respective treatment equipment. In the front portion of the room where transportation vehicle is parked for unloading, the floor shall be made impermeable so that any liquid spillage during unloading does not percolates into the ground. The liquid generated during handling of wastes and washing, shall be diverted to the inlet

of effluent treatment plant (ETP). In the main storage room, wastes shall be stacked with clear distinction as per the color coding of the containers by providing partitions. From here, the colored containers may be sent to the respective treatment equipment by using suitable closed type of conveyance (trolley etc.,). The main storage room too shall have provisions similar to that of equipment room such as roofing, well ventilated, easy to wash floors & walls, smooth and fine surfaces etc.

Apart from the above, a CBWTF should have separate storage provision for storage of mercury bearing waste collected from the member health care facilities as per the procedure given in CPCB guidelines. Mercury storage provision should be provided as per the guidelines issued by CPCB (refer www.cpcb.nic.in). The capacity of the mercury storage provision should be maximum of 90 days and by which the collected mercury bearing waste shall have to be disposed of through a TSDF located nearby following the manifest as per Hazardous and Other Waste (Management and Transboundary Movement) Rules, 2016. The charges for collection and disposal of mercury bearing waste shall be collected by the CBWTF from the respective member HCF.

c) Treated waste storage room

Separate space should be provided to store the wastes treated in different treatment units. The wastes shall be stored in separate group as per the disposal options. Other provisions in the room shall be similar to the main storage room. Waste such as incineration ash/vitrified ash generated in the process of incineration/plasma pyrolysis respectively shall be stored safely in a separate area under the shed so as to avoid entry of rain water during the monsoon and for easy collection. In case, incineration ash/ vitrified ash is found to be hazardous waste in nature same should be disposed of through any authorized TSDF operator located nearby following the manifest as per Hazardous and Other Waste (Management and Transboundary Movement) Rules, 2016. In case of a State/UT where TSDF is not available, all the CBWTF operators have to store incineration ash safely as per these guidelines.

d) Administrative Room

This room shall be utilized for general administration, record keeping, billing etc.

e) Generator set

CBWTF shall have a generator set of adequate capacity as standby arrangement for power, with sufficient capacity to run the treatment equipment during the failure of power supply. The generator set shall comply with the necessary requirement as per DG Set norms notified under the Environment (Protection) Act, 1986.

f) Continuous emission monitoring system (CEMS)

Monitoring provision for continuous monitoring of the incinerator/plasma pyrolysis stack emission shall be installed by the CBWTF operators for the parameters as stipulated by the respective SPCB/PCC as per the authorisation granted under the BMW Rules, 2016. Other-wise, at present, all the existing CBWTF operators are required to carry out stack emission monitored using continuous emission monitoring system for the flue gas parameters such as CO₂, O₂, CO as well as primary & secondary chamber temperatures, and records maintained. The continuous emission monitoring system for stack emission should be installed as per the guidelines issued by SPCB/PCC/CPCB. Also, the real time continuous stack emission monitoring data is also required to be transmitted to the servers of the respective SPCB/PCC as well as CPCB, by all the existing CBWTF operators

g) Vehicle Parking

Provision for parking shall be made within the confines of the site for parking of required number of vehicles, loading and unloading of the vehicles meant for transporting waste to and from the facility, etc. In case of a CBWTF with space constraints, multi-storey parking or a separate provision may be allowed only for parking of vehicles.

h) Display and sign board

An identification board (Display) of durable material and finish shall be displayed at the entrance to the facility. This shall clearly display the name of the facility, owner name, address and telephone number of the operator and the prescribed authority, no. of hours of operation & operational hours, telephone numbers of the personnel to be contacted in the event of an emergency, validity period of authorization as well as total daily waste treated and disposed. Also, sign boards should be provided at all the salient points (untreated waste storage area, treatment equipment, treated waste storage area, ETP, firefighting equipment) within the facility.

i) Washing Room

A washing room shall be provided for eye washing/hand washing/ bathing etc. for the workers.

j) Site Security

High walls, fencing and guarded gates shall be provided at the facility to prevent unauthorized access to the site by humans and livestock.

k) Fire safety

Fire safety equipment such as sand buckets and fire extinguishers should be provided at all the salient points of the CBWTF including at the diesel storage areas, diesel tanks connected with the incinerator etc. Fire alarm also should be provided within the CBWTF to prompt the workers in the event of any fire hazard. Workers should also be trained in First Aid administration.

l) First Aid Box

First Aid Box with necessary provisions need to be provided at all the salient points within the facility.

m) Green Belt

The open area available within the CBWTF shall be developed into green belt.

n) Website:

All CBWTFs shall develop own website and the upcoming CBWTF shall develop the website prior to the commencement of the facility. The website should be uploaded with relevant information periodically (on monthly basis) especially as detailed below:

- (i) A copy of the Environmental Clearance obtained;
 - (ii) Copies of the Consents under the Water (Prevention and Control of Pollution) Act, 1974 and Air (Prevention and Control of Pollution) Act, 1981 as well as the Authorisation under the BMW Rules obtained from the SPCB/PCC;
-

-
- (iii) List of all the member Health Care Facilities with complete address, bedded or non-bedded HCFs, no. of beds, bar code, category-wise average bio-medical waste generation in kg/annum;
 - (iv) Charges levied on the member Health Care Facilities (HCFs) for treatment and disposal of bio-medical waste;
 - (v) Vehicles connected with a provision of GPS as per BMW Rules and Vehicle-wise route chart for collection, transportation of bio-medical waste from the member HCFs;
 - (vi) Real time continuous online stack emission monitoring data;
 - (vii) Monthly details of total waste collected from the member HCFs, total waste treated, and treated recyclable plastic waste or glass waste sold to the parties and final mode of disposal of incineration ash;
 - (viii) A copy of the annual report submitted to the respective SPCB/PCC;
 - (ix) Monitoring results of the stack emissions, treated wastewater and incineration ash, as per the frequency stipulated under the BMW Rules;
 - (x) List of HCFs (located within the coverage area) with complete address which have not taken membership of the CBWTF for disposal of Bio-medical waste;
 - (xi) Contact person, contact telephone number and e-mail addresses of the facility; and.
 - (xii) Provision to have access to the SPCB/PCC/CPCB/MoEF & CC/MoH & FW especially on GPS, online monitoring system and the data.

Besides the provisions suggested in the earlier paras, following important provisions should also be made in a CBWTF:

- (i) A telephone shall be provided and maintained at the facility.
 - (ii) A First Aid Box shall be provided and maintained at the CBWTF.
 - (iii) Proper lighting shall be provided at the facility.
 - (iv) Proper care shall be taken to keep the facility and surroundings free from odors.
 - (v) Measures shall be implemented to control pests and insects at the site.
 - (vi) Measures shall be implemented to control the escape of litter from the site.
 - (vii) Necessary provision shall be made to prevent and control noise generated, if any, due to the activities at the site.
 - (viii) Necessary protective gear for the waste handlers shall be provided.
 - (ix) Immunization to all the workers of CBWTF against all the diseases including especially Tetanus and Hepatitis -B as stipulated under the BMW Rules.
 - (x) Workers should have provisions such as washing, toilet, and suitable place for eating.
-

- (xi) Workers should also be provided with N-95 mask besides other PPEs such as hand gloves, gumboots, goggles etc.

Every CBWTF operator shall submit a work-plan to the Prescribed Authority. The work-plan should include the details of facilities at the CBWTF, collection, transportation & storage of the bio-medical wastes, operational details etc.

11) Record keeping

Maintenance of records for all operations carried out at the CBWTF is very important to monitor overall operation of the CBWTF. It also helps in submission of the required information to be submitted to the 'Prescribed Authority' by 30th June of every year as per the format prescribed under the BMWM Rules or provided by the SPCB/PCC. A well-maintained record of all the activities at the CBWTF also enables the facility operator to produce all information of the activities on demand of the concerned prescribed authority. The record should include all information relating to each activity at the CBWTF site as per BMWM Rules which include accidents occurred (spills, injury, fire accident) and the measures taken and also, however, minimum requirement is outlined below:

a) Records of waste movements

Daily records shall be maintained for the waste accepted and treated waste removed from the site. This record shall include the following minimum details:

- (i) **Waste accepted:** -Records on day-to-day basis (as per the format given at **Annexure-II**) shall be maintained with respect to the waste collection date, name of the healthcare unit with bar code, waste category as per BMWM Rules, category-wise quantity of waste accepted, vehicle registration number used for collection of bio-medical waste from member health care facilities, time at which waste collected from member HCFs, name of the vehicle driver and his signature and waste receiving date & time (at CBWTF site). Similar information to be acknowledged to the member health care facility by the CBWTF operator on daily basis.
- (ii) **Treated waste to be disposed :-** Date, treated waste type, Quantity, vehicle number, disposal as stipulated under BMWM Rules.

b) Logbook for the treatment equipment

A logbook shall be maintained for each treatment equipment installed at the site and shall include the following:

- (i) The weight of each batch.
- (ii) The categories of waste as per the Rules.
- (iii) The time, date and duration of each treatment cycle and total hours of operations.
- (iv) The complete details of all operational parameters during each cycle.

Log book to be maintained for operating the incinerator/plasma pyrolysis as well as the autoclave as per the formats given at **Annexure –III.**

c) Monitoring and reporting of operations in the CBWTF:

The monitoring of the key operating parameters of treatment equipment provides several benefits. First, monitoring provides the operator with information needed to make decisions on necessary combustion control adjustments. Second, properly maintained monitoring records can provide useful information for identifying operating trends and potential maintenance problems. Following are the suggested parameters for monitoring of the treatment equipment

(i) Monitoring of operating parameters of the incinerator/plasma pyrolysis:
Following operating parameters can be monitored in case of incinerator/plasma pyrolysis:

- Waste charge rate.
- Combustion gas temperature in primary and secondary chamber as well as the temperature of the stack exit gas (flue gas).
- Condition of the draft (negative draft in primary chamber).
- Combustion gas oxygen level in primary and secondary chamber as well as stack exit gas.
- Air flow rate through the incinerator/plasma pyrolysis.
- Carbon-Di-Oxide (CO₂), Oxygen (O₂) and Carbon Monoxide (CO) level in the flue gas.

-
- Quantity of auxiliary fuel usage as well as the power consumption (in every batch).
 - Pressure drop in the primary chamber and APCD attached with the incinerator/plasma pyrolysis and
 - Bottom ash or slag quality (for Total Organic Carbon (TOC) as well as loss on ignition and the hazardous constituents (at least once in a quarter).

(ii) **Monitoring of operating parameters of the Autoclave:** Following operating parameters can be monitored during the sterilization using autoclave:

- Time at which sterilization started and time at which sterilization completed.
- Temperature conditions maintained throughout the sterilization
- Conditions of pressure maintained throughout the sterilization
- Duration of sterilization
- Validation test results

Records concerning the above parameters need to be maintained and checked periodically for taking remedial measures during the operation of the incinerator or plasma pyrolysis or autoclave. In case of other treatment processes, the operational conditions as well as the efficacy tests to be complied with as per the standards prescribed under the BMWM Rules.

(iii) **Frequency of monitoring:**

The CBWTF operator shall carry out following tests through a NABL approved laboratory or a laboratory approved under the Environment (Protection) Act, 1986, as per the frequency stipulated under the BMWM Rules or as prescribed by the SPCB/PCC and record of such analysis results shall be maintained and submitted to the prescribed authority (SPCB/PCC), as suggested below:

- **Liquid effluent:** Parameters such as pH, Suspended Solids, Oil & Grease, BOD, COD, Bio-assay for liquid effluent being discharged from the CBWTF be monitored as per the Consent conditions or once in a quarter and such records maintained and submitted to SPCB/PCC.
 - **Stack emission monitoring:**
-

In case of the BMW incinerators, the Stack Emission shall be monitored (under optimum capacity) for parameters such as Particulate Matter, HCl, NO_x, Hg & compounds and combustion efficiency once in three months as required under schedule II of the Bio-medical Waste Management Rules 2016 (All monitored values shall be corrected to 11% Oxygen on dry basis). In case of dioxins and furans, monitoring should be done once in a year (monitored values shall be corrected to 11% Oxygen on dry basis).

➤ **Validation test of autoclave/microwave/chemical treatment/Dry heat sterilization:**

Suggested validation test for treatment of bio-medical waste by autoclave/microwave/chemical treatment/Dry heat sterilization is given in **Table 1**.

Table 1: Suggested validation test for treatment of bio-medical waste by autoclave/microwave/chemical treatment/Dry heat sterilization

S. No	Type of equipment used for treatment of bio-medical waste	Type of Validation Test	Frequency
(i)	Autoclave	(i) biological indicator strips or vials Geobacillus stearothermophilus spores with at least 1×10^6 spores),	once in three months
		(ii) chemical indicator strip or tape	each batch of waste treated
(ii)	Microwave	Bacillus atrophaeus spores using vials or spore strips with at least 1×10^4 spores per detachable strip	Recommended: once in three months
(iii)	Chemical treatment followed by shredding	Bacillus Subtilis (ATCC 19659)- 4 Log10 reduction or greater	Once in a week
(iv)	Dry heat sterilization	consistently kill the biological indicator Geobacillus Stearothermophilus or	Once in three months

S. No	Type of equipment used for treatment of bio-medical waste	Type of Validation Test	Frequency
		Bacillus Atropheaus spores using vials with at least 6 log ₁₀ spores per ml.	
		A chemical indicator strip or tape	Once in a week

d) Site Records:

Site records shall include the following:

- (i) All the approvals obtained from other concerned departments other than the prescribed authority;
- (ii) Details of construction or engineering works;
- (iii) Maintenance schedule, breakdowns/trouble shootings and remedial actions;
- (iv) Emergencies;
- (v) Incidents of unacceptable waste received and the action taken; and
- (vi) Details of site inspections by the officials of the regulatory authorities, purpose of visits with date and necessary actions initiated on the observations.

Daily, monthly and annual summary records of all the above shall be maintained and made available at the site for inspection and same submitted whenever required by an authorized official of the concerned regulatory authorities.

12) Collection and transportation of bio-medical waste

The collection and transportation of bio-medical waste shall be carried out in a manner so as to prevent any possible hazard to human health and environment. Collection and transportation are the two operations where the chances of segregated bio-medical waste coming in contact with the public, rag pickers, animals/birds, etc. are high. Therefore, all care shall be taken to ensure that the segregated bio-medical waste handed over by the healthcare units reach CBWTF without any damage, spillage or unauthorized access by public, animals etc. A responsible person from the CBWTF operator shall always accompany the vehicle to supervise the collection and transportation of bio-medical waste. Also, the private transport vehicles should not be

authorised by the SPCBs/PCCs only for transportation of the Bio-medical Waste. The CBWTF operator should be made responsible for collection and transportation of bio-medical waste.

a) Collection of bio-medical waste:

Generator of the bio-medical waste is responsible for providing segregated waste in accordance with the provisions of the Bio-medical Waste Management Rules, 2016, to the CBWTF operator. Dedicated temporary storage at healthcare unit shall be designated. The coloured bags handed over by the healthcare units shall be collected in similar coloured containers with proper cover. Each bag shall be labeled as per Schedule IV of the Bio-medical Waste Management Rules as well as with bar coding system (to be complied by the occupier or operator of a CBWTF as per BMWM Rules) so that at any time, the healthcare units can be traced back that are not segregating the bio-medical wastes as per BMWM Rules. The coloured containers should be strong enough to withstand any possible damage that may occur during loading, transportation or unloading of such containers. These containers shall also be labeled as per Schedule IV of the Rules. Sharps shall be collected in puncture resistant container. The person responsible for collection of bio-medical wastes shall also carry a register with him to maintain the records such as name of the healthcare unit, the type and quantity of waste received, time at which waste collected from the member HCF, signature of the authorised person from the healthcare unit etc. During transportation, the containers should be covered in order to prevent exposure of public to odours and contamination.

(b) Transportation of the collected bio-medical waste to the CBWTF:

All the vehicles used by the CBWTF operator shall not be sub-letted or contract vehicles should not be used by the CBWTF operator. All the vehicles owned by the CBWTF operator and intended only for collection of bio-medical waste from the member health care facilities should be registered under the Motor Vehicle Act with the respective RTO/Transport Department and such vehicle numbers should also be registered with the respective SPCB/PCC for the purpose of collection of bio-medical waste from the member health care facilities. The bio-medical waste collected in designated coloured containers shall be transported to the CBWTF in a fully covered vehicle. Such vehicle shall be dedicated for transportation of bio-medical waste only. Depending upon the volume of the wastes to be transported, the vehicle may be a

two or three-wheeler, light motor vehicle or heavy duty vehicle. In either case, the vehicle must possess the following:

- (i) Transportation vehicle shall be fitted with GPS to track the movement of the vehicle.
 - (ii) Separate cabins shall be provided for driver/staff as well as for placing the designated colour coded bio-medical waste containers.
 - (iii) Two wheeler registered under the Motor Vehicle Act shall be permitted for collection of bio-medical waste only from the clinics or dispensaries located in places where the lanes are narrow and not easily accessible to four wheeler vehicles. Such two wheeler vehicle (s) should have a provision of a suitable fixed waste collection box marked with bio-hazard symbol, contact details, proper lid, emergency spill collection procedure, first aid box and manifest record in accordance with the BMWM Rules
 - (iv) The base of the waste cabin shall be leak proof to avoid pilferage of liquid during transportation.
 - (v) The waste cabin may be designed for storing waste containers in tiers and also should be provided with a lighting provision.
 - (vi) The waste cabin shall be so designed that it is easy to wash and disinfect.
 - (vii) The inner surface of the waste cabin shall be made of smooth surface to minimize water retention.
 - (viii) The waste cabin shall have provisions for sufficient openings in the rear and/or sides so that waste containers can be easily loaded and unloaded.
 - (ix) The vehicles used for the purpose of collection and transportation of bio-medical waste must be labelled with the bio-hazard symbol (as per Schedule IV of the BMWM Rules, 2016) in red/black colour and should display the name, address, and contact number of the CBWTF operator in green colour. CBWTF authorized by (*"Name of SPCB/PCC"*) shall also be mentioned below name,
-

address and contact number of the CBWTF operator in green colour, as given in **Annexure-VII**.

- (x) All the existing vehicles used for the purpose of collection and transportation of biomedical waste shall be labelled with the bio-hazard symbol and shall display the name, address, and contact number of the CBWTF operator on white background (as given in **Annexure-VII**). Further, vehicles registered with the respective SPCB/PCC for the purpose of collection and transportation of biomedical waste after June, 2025 shall be white in colour.
- (xi) Bio-hazard symbol size and font size shall be in minimum proportion of 12:3 and 12:1, respectively, with respect to body height of the vehicle used for transportation of biomedical waste. For Example: If body height is 6 feet i.e. 72" then minimum font size will 6" and minimum size of bio-hazard symbol will be 18" as given in **Annexure-VII**.
- (xii) The vehicle driver should carry always valid registration of the vehicle obtained from the concerned transport authority and also carry valid 'pollution under control certificate' issued by the authorized certificate issuing agency.

Depending upon the area to be covered under the CBWTF, the route of transportation shall be worked out. The transportation routes of the vehicle shall be designed for optimum travel distance and to cover all member healthcare units of the CBWTF. The CBWTF operator should ensure online and real time tracking & monitoring provisions (GPS provision) should be given access with passwords to the SPCB/PCC and CPCB to cross check the movement of the transportation vehicles on any time by the SPCB/PCC/CPCB. As far as possible, the transportation shall be carried out during non-peak traffic hours. If the area to be covered is very large, a satellite station may be established to store the bio-medical waste collected from the adjoining areas. The wastes so stored at satellite station may then be transported to the CBWTF in a big vehicle. It shall be ensured that the total time taken from generation of bio-medical waste to its treatment, which also includes collection and transportation time, shall not exceed 48 hours.

13) Disposal option of solid waste generated from the CBWTF

Treated plastic waste, incineration ash, treated waste sharps and glass waste, Oil & Grease waste and ETP sludge are generally generated from the CBWTF from the treatment systems such as autoclaving/microwaving, incineration, chemical disinfection and effluent treatment plant respectively. The treated bio-medical waste shall be disposed as per the options suggested in the **Table 2** given below:

Table 2: Suggested Disposal option of solid waste generated from the CBWTF

Sl. No.	Treated Waste Category	Suggested Treatment and Disposal Options
1.	Plastic wastes	Plastic waste should not be sent to landfill sites. Plastic waste after disinfection and shredding, is required to be (i) sent to registered or authorized recyclers (or) (ii) for energy recovery (or) (iii) diesel or fuel oil recovery (or) (iv) for road making, whichever is possible.
2.	Disinfected Sharps (including needles and syringes)	Treatment by Autoclaving or Dry Heat Sterilization followed by shredding or mutilation or combination of shredding cum autoclaving. Treated sharps need to be disposed of (i) by encapsulation in metal container or cements concrete; (or) (ii) sent for final disposal to iron foundries (having consent to operate from the SPCBs/PCCs) (or) (iii) Disposal in sanitary landfill; (or) (iv) Disposal in designated concrete waste sharp pit.
3.	Incineration ash	Incineration ash from incineration of any bio-medical waste shall be disposed through hazardous waste treatment, storage and disposal facility (TSDF), if toxic or hazardous constituents are present beyond the prescribed limits as given in Schedule –II of the Hazardous and Other Waste Management & Transboundary Movement Rules or as revised from time to time.
4.	Other treated solid wastes like Glass waste	Disinfection (by soaking the washed glass waste after cleaning with detergent and Sodium Hypochlorite

Sl. No.	Treated Waste Category	Suggested Treatment and Disposal Options
		treatment) or through autoclaving or microwaving or hydroplaning and then sent for recycling.
5.	Oil & Grease	By Incineration
6.	ETP Sludge	After drying in sludge drying beds or removal of moisture content using 'Filter Press' and such ETP sludge shall be given to CBWTF for incineration or to the hazardous waste treatment, storage and disposal facility (HWTSDf) for disposal in Secured Landfill
7.	Hazardous Waste	Disposal through a TSDF located nearby following the manifest as per the Hazardous and Other Waste (Management & Transboundary Movement) Rules, 2016

14) Cost to be charged by the CBWTF Operator for the Health Care Facilities

Cost to be charged from the healthcare facilities plays an important role in financial viability and sustainable operation of a CBWTF project, for providing the best treatment services to the Health Care Units and for ensuring compliance to the BMWM Rules. The cost shall be so worked out that neither it becomes a monopoly of the CBWTF operator nor the interest of the CBWTF operator is overlooked. It is recommended that cost to be charged from the healthcare units, depending on the size, no, of beds and the distance from the location of the CBWTF and same shall be worked out in consultation with the concerned SPCB/PCC and the local Medical Association, keeping in view the following options:

- (a) In case of non-bedded health care units, fixed charges depending on the average quantity of waste generation per day, in case of the nursing homes/clinics/sample collection Centres /Dental HCentres, dispensary, pathological laboratory, blood banks, and other non-bedded hospitals irrespective of their system of medicine including ayush hospitals.
- (b) In case of bedded hospitals, fixed charges per bed per day basis and based on the no. of beds for which consents under the Water Act, 1974/Air Act, 1981 and authorization granted under the BMWM Rules, by the prescribed authority

Note:

- (i) *Rates are required to be revised once in a year based on the Wholesale Price Index (WPI Index) or Consumer Price Index (CPI Index) (considering the prevailing market price especially in respect of the labour expenses, diesel prices, electricity, operating cost etc.), by the State Advisory Committee in consultation with the concerned SPCB/PCC, local Medical Association and the representatives of the CBWTF Association*
- (ii) *The Health Care Facilities are required to ensure timely payments to the CBWTFs for ensuring timely treatment services in compliance to the BMWWM Rules as well as agreement made with the concerned CBWTF Operator.*

15) Check list for development of CBWTF

The criteria for development of CBWTF have been discussed in detail in the Previous sections. However, to have at a glance check in developing CBWTF, checklist is reproduced for convenience and is annexed **(Annexure-IV)**.

16) Periodic inspection/monitoring or performance evaluation of the CBWTF

To have uniformity in performance evaluation of the CBWTF throughout the country, a check list for performance evaluation of the CBWTF for carrying out inspection/monitoring/compliance verification has been prepared and is annexed **(Annexure –V)**. All the prescribed authority (SPCB/PCC) shall inspect the CBWTF at least once in six months located in the respective State/UT and a copy of the inspection reports shall be submitted to CPCB and MoEF & CC along with a copy of the action taken for ensuring compliance to the BMWWM Rules and CPCB guidelines issued from time to time and also such information is required to be uploaded in SPCB/PCC website. CPCB shall carryout random inspection of the CBWTFs once in a quarter and any violations observed further actions shall be initiated by CPCB if required under the Environment (Protection) Act, 1986.

-- OO -

Appendix-I**Methodology to Conduct gap analysis with respect to generation and treatment of biomedical waste - Revision 1**

Guidelines for Common Biomedical Waste Treatment Facilities was prepared by CPCB with an aim to have uniformity in ensuring site selection, allowing and establishment of a state-of-the-art Common Biomedical Waste Treatment Facilities (CBWTFs), operation as well as verification of compliance to the BMW Rules, 2016 throughout the country. As per the said guideline, SPCB/PCC is required to prepare an inventory or review with regard to the bio-medical waste generation at least once in five years in the coverage areas of the existing CBWTF and conduct gap analysis as per format given in Annexure-I of the guideline.

Further, methodology for conducting gap analysis with respect to generation and treatment of biomedical waste prepared by CPCB and circulated to all SPCBs/PCCs. Accordingly, 12 SPCBs/PCCs have conducted gap analysis and submitted the report to CPCB. However, non-uniformity and ambiguity was observed specifically with regard to the method for extrapolating the data on biomedical waste generation and requirement of adequate treatment capacity in the gap analysis reports submitted by SPCBs/PCCs. Therefore, revised methodology have been prepared with an aim to have uniformity in the method for carrying out the gap analysis by State Pollution Control Boards/Pollution Control Committees.

The methodology for conducting gap analysis may be based on following parameters:

S. No.	Parameters	Details
1.	Coverage area of CBWTF	Mention farthest distance covered by CBWTF
2.	No. of HCFs (Bedded and non-bedded)	In Number
3.	No. of Beds covered	In Number
4.	Total biomedical waste generation (in Kg/day)	The generation of biomedical waste may be calculated by considering following aspects: a) Generation from bedded HCFs: The biomedical waste generation rate may be considered as 277* grams per bed per day

		b) Generation from non-bedded HCFs: The biomedical waste generation may be considered as 274** grams per day c) Biomedical waste generated from occasional waste generators such as health camps, institutions, vaccination camps etc as defined under CPCB guidelines may also be considered. * Reference: Report on Health-care Waste Management status in countries of the South-East Asia Region by WHO which is also nearly equal to the average biomedical waste generation per day per bed as per AR information received from States/UTs. **The value is taken based on the data given by CBWTF Associations regarding current average biomedical waste generation from non-bedded HCFs.
5.	Extrapolate the biomedical waste generation for next 10 years	Linear method may be adopted for extrapolation of biomedical waste generation
6.	Total existing treatment capacity (in Kg/day) (Sum of Incineration Capacity and Autoclave/Microwave/Hydroclave Capacity)	For calculation of existing treatment capacity, maintenance time (not more than 12-18 hrs/month) may be considered for calculating operational hours of equipment as below: a) Operational Hours for static incinerator 20 hrs/day b) Operational hours for Rotary incinerator 22 hrs/day c) 18 cycle per day for autoclave

		The actual capacity may also be considered as 90% of available capacity keeping 10% margin for diverted/extra waste etc.
7.	Total Biomedical Waste treated and disposed (Kg/day)	Sum of all categories of biomedical waste treated and disposal.
8.	Gap between total extrapolated biomedical waste generation (for next 10 years) and existing biomedical waste treatment capacity	Extrapolated biomedical waste generation minus total existing treatment capacity

Annexure-I**Coverage area-wise gap analysis for assessing additional BMW treatment capacity requirement**

S. No	Coverage area (pl. indicate areas covered by a CBWTF in the State/UT)	No. of HCFs		No. of Beds covered	Total estimated BMW generation in Kg/day	Total existing treatment capacity in Kg					Total BMW Treated and Disposed in Kg/day	Gap between total BMW Generation and the Existing BMW Treatment Capacity in Kg	Remarks (Whether additional Treatment Capacity is required or not)	
		Bedded	Non-bedded			Incineration	Autoclaving/ Hydroclaving /microwaving	Chemical disinfection	Deep burial	Any other mode of disposal			Yes	No
(1)	(2)	(3)	(4)	(5)	(6)	(7)	(8)	(9)	(10)	(11)	(12)	(13)	(14)	(15)

Note: Above gap analysis coverage area-wise is required to be prepared once in five years and should be shown or depicted in a Map of State/UT.

Format for maintaining the records by the CBWTF Operator alongwith the transportation Vehicle used for collection of bio-medical waste from the member HCFs

Name of the CBWTF	:
Address of the CBWTF with contact details	:
Vehicle Registration Number (certificate to be carried by the vehicle driver)	:
Route covered (indicate places) by the vehicle	:

Note: Above format is required to be maintained in duplicate both by the CBWTF Operator and the member HCF

[illegible]

Log book for Operating the Incinerator/Plasma Pyrolysis

[illegible]

Note: Fill the details whichever is applicable

Log Book for Operating the Autoclave/Hydroclave

[illegible]

Annexure – IV

Check List for Development of a Common Bio-medical Waste Treatment and Disposal Facility & For issuing 'Consent to Establishment under Water & Air Acts

-
1. Name of the Proponent :
 2. Proposed location of the CBWTF :
 3. No. of HCFs in the locality :
 4. No. beds :
 5. Total Bio-medical Waste Generation in kg/day :
 - (i) Incinerable in kg/day :
 - (ii) Autoclavable in kg/day :
 - (iii) Glass waste in kg/day :
 - (iv) Waste sharps in kg/day :
 6. **Proposed location of the CBWTDF:** located away from
 - a) Residential area : Yes ☐ No ☐
 - b) Sensitive area : Yes ☐ No ☐
 - c) Industrial area : Yes ☐ No ☐
 - d) Is it as a part of TSDF : Yes ☐ No ☐
 - e) Is the facility proposed in Hilly areas: Yes ☐ No ☐
 - d) Buffer distance of 500 m available : Yes ☐ No ☐
 7. **Proposed land area for CBWTF:**
 - a) Area about 1 acre : Yes ☐ No ☐
 - b) Area less than 1 Acre : Yes ☐ No ☐
 - c) Area more than 1 Acre : Yes ☐ No ☐
 8. **Proposed coverage area of the CBWTF:**
 - a) Any facility located upto a radius of 75 KM from the proposed locality : Yes ☐ No ☐
 - b) No. of beds covered by the existing facility/proposed facility:
 - (i) more than 10, 000 beds : Yes ☐ No ☐
 - (ii) less than 10,000 beds : Yes ☐ No ☐
 - c) Is there any CBWTF within the radius of 75 KM : Yes ☐ No ☐
 - d) BMW Waste generation in a coverage area under consideration: Kg/day
-

- e) Existing CBWTF treatment Capacity :
- (a) Incineration/plasma pyrolysis :..... Kg/day
- (b) Autoclave/hydroclave :Kg/day
- (c) Chemical Disinfection :..... Kg/day
- f) Is locality requires any additional capacity (within a radius of 75 KMs)?.
- : Yes ☐ No ☐
- (i) If so, indicate reason:.....

9. Requirement of Treatment Facility: Following treatment facilities shall be provided in a CBWTF:

- a) Incineration : Yes ☐ No ☐
- b) Autoclave (Pre-vacuum horizontal feeding) / Hydroclave / Microwave. : Yes ☐ No ☐
- c) Shredder : Yes ☐ No ☐
- d) Sharp pit (with drawing details) : Yes ☐ No ☐
- e) Provision for floor washing/vehicle washing: Yes ☐ No ☐
- f) Effluent Treatment Plant : Yes ☐ No ☐
- g) Secured land fill/Disposal of ash in TSDF : Yes ☐ No ☐
- h) Other provisions as per CPCB guidelines : Yes ☐ No ☐

10. Segregation

- (i). Segregation shall be as per the Bio-medical Waste Management Rules, 2016 as amended as well as compatible with treatment facilities at CBWTF
- (ii). Occupier/Generator is responsible for providing segregated waste to the operator.

11. Collection

- (i) Respective coloured bags provided with bar code should be kept in similar coloured container i.e. coloured bags shall not be directly kept in vehicle.
- (ii) Sharps shall be collected in puncture resistant, leak proof, rigid containers.
- (iii) Temporary storage at healthcare unit shall be designated.

12. Transport Vehicle

-
- (I) Dedicated vehicles for collection of Bio-medical waste : Yes ☐ No ☐
 - (II) Separate cabins shall be provided for driver/staff and the bio-medical waste containers : Yes ☐ No ☐
 - (III) The base of the waste cabin shall be leak proof to avoid pilferage of liquid during transportation : Yes ☐ No ☐
 - (I) The waste cabin may be designed for storing waste containers in tiers : Yes ☐ No ☐
 - (V) The waste cabin shall be so designed that it is easy to wash and disinfect. : Yes ☐ No ☐
 - (VI) The inner surface of the waste cabin shall be made of smooth surface to minimize water retention : Yes ☐ No ☐
 - (VII) The waste cabin shall have provisions of sufficient openings in the rear and/or sides so that waste containers can be easily loaded and unloaded : Yes ☐ No ☐
 - (VIII) The vehicle shall be labeled with the bio-hazard symbol (as per Schedule IV of BMW Rules) and should display the name, address and telephone number of the CBWTF : Yes ☐ No ☐
 - (IX) Other provision as per CPCB guidelines : Yes ☐ No ☐

13. Storage

- (I) Sufficient ventilated storage space for untreated and treated bio-medical waste shall be provided. : Yes ☐ No ☐
- (II) The flooring and walls (to a height of 2M from floor) shall be finished with smooth and fine material. There shall be minimum number of joints. : Yes ☐ No ☐

14. Record Keeping

- (I) Documents such as collection advice taken from health care units for each category of waste, records of waste movements, logbook for the equipment and site records shall be maintained. : Yes ☐ No ☐
- (II) All the record (five year) shall be available at the CBWTF site for inspection. : Yes ☐ No ☐

15. Proposed Treated Waste Disposal method:

- (i). Incineration ash - Secured landfill/near by TSDF : Yes ☐ No ☐
-

- (ii). Plastic waste after disinfection and shredding –Registered Recycling Unit
: Yes ☐ No ☐
- (iii). Sharps, after disinfection (if encapsulated) - Municipal landfill
: Yes ☐ No ☐
- (iv). Treated wastewater –Discharge into sewer/drain or recycling in APCD
: Yes ☐ No ☐
- (v). Oil & grease –By incineration: Yes ☐ No ☐
- (VI). Any other mode of disposal of recyclable waste:
(If so, pl. indicate)

16. Estimated energy consumption and fuel consumption per month :

- (i) Estimated energy consumption per month
- (a) General lighting in the facility :
(b) Incinerator :
(c) Autoclave/microwave :
(d) Shredder :
(e) ETP :
(f) Any other :
- (ii) Estimated fuel consumption:
- (a) Diesel consumption :..... in KI per month
(b) No. of hours of operation of DG Set :
(c) No. of hours of incineration :

17. Whether the proponent obtained necessary approvals from the concerned departments as required : Yes ☐ No ☐

(i) If yes, attach details

18. Whether the proponent obtained EC as per EIA 2006 and the amendments made thereof : Yes ☐ No ☐

(i) If yes, attach a copy of the EC obtained from the concerned

19. Whether the proposal recommended for issuing consent to establish

: Yes ☐ No ☐

(Signature of the official verified with date)

Annexure – V

**Check List for Performance Evaluation of the
Common Bio-medical Waste Treatment and Disposal Facility (CBWTF)**

S.No.	Details		Particulars
01.	Name of CBWTF with contact details	:	
02.	Date of visit	:	
03.	Location details of the CBWTF	:	a) Near to Residential area: :Yes ☐ No ☐ b) In/near Sensitive area: Yes ☐ No ☐ c) In Industrial area : Yes ☐ No ☐ d) Is there a buffer zone of 500 m: Yes ☐ No ☐ Indicate exact distance: in KM e) Is it as a part of TSDF: Yes ☐ No ☐ If so, distance of TSDF from the nearest CBWTF:KM.. f) Is the facility proposed in Metropolitan city: Yes ☐ No ☐ (i)Name of the City: (ii)Population of the City (as per latest census): g) Is the facility proposed in Hilly area : Yes ☐ No ☐ (i)Name of the Town/City:
04	Month / year of establishment and the Consents status	:	Establishment Month/Year :
05.	CBWTF set up by	:	
06.	CBWTF operated by	:	
07.	Total number of healthcare facilities and beds covered (as on date of visit)	:	No. of HCFs : No. of Beds : No. of HCFs and beds upto 75 KM radius:

S.No.	Details		Particulars
08.	Total BMW Treatment Capacity of CBWTF (in kg / day)	:	Incineration : Autoclave : Chemical Disinfection: Any other treatment and disposal:
09.	Consents and Authorization details :		
9.1	Consent under Water (Prevention and Control of Pollution) Act, 1974	:	☐ Applied for ☐ Not Applied for ☐ Possess Valid Consent ☐ Not renewed ☐ No consent If obtained: Consent is valid upto and issued bySPCB/PCC vide letter dated
9.2	Consent under Air (Prevention and Control of Pollution) Act, 1981	:	☐ Applied for ☐ Not Applied for ☐ Possess Valid Consent ☐ Not renewed ☐ No consent If obtained: Consent is valid upto and issued bySPCB/PCC vide letter dated
9.3	Environmental Clearance (EC)		☐ Applied for ☐ Not applied ☐ Obtained ☐ Not obtained If obtained: EC issued by SEIAA or MoEF& CC vide letter dated
9.4	Authorization under BMW Rules, 1998	:	☐ Applied for ☐ Not Applied for ☐ Possess Valid Authorisation ☐ Not renewed ☐ No Authorisation If obtained: Authorisation is valid upto and issued bySPCB/PCC vide letter dated
10.	Investment in setting up the CBWTF	:	
11.	Area of plot size for CBWTF (Sq. ft.)	:	
12	Annual Report submission for the year	:	Submitted before due date : :Yes ☐ No ☐ If yes, provide details of waste collected, received and treated & disposed of:
12.	Coverage area of CBWTF (radius in KM covered)	:	Coverage area upto 75 km radius: Yes ☐ No ☐

S.No.	Details		Particulars
13.	Name of Districts/Cities / places being covered	:	(Pl. indicate Districts or places covered:.....) W.r.to the CBWTF (i) Farthest HCF located at :KM (ii) Nearest HCF located at :KM.
14.	Daily operation schedule (timings)	:	(i) Collection: ...AM to ... PM. (ii) Incineration:....AM to ...PM (iii) Whether waste from member HCFs collected in holidays: ☐ Yes ☐ No
15.	Cost charged to the healthcare facilities	:	(i) Charges in Rs..... (ii) Is the cost to be levied suggested by:Organisation
16.	Total quantity of bio-medical waste treated: kg/day (avg.)		
16.1	Incinerable	:	 %
16.2	Autoclaving	:	%
16.3	Chemical Disinfection	:	%
16.4	Others (please specify waste type-wise)	:	%
17.	Staff involvement in CBWTF operation (number of persons):		
17.1	Managerial / Administration	:	
17.2	Equipment operations	:	
17.3	Transportation of BMW	:	No. of Drivers: No. of Helpers:
17.4	Sanitation and others	:	
17.5	Total persons excluding managers	:	
18.0	Collection and Transportation of bio-medical waste from member HCFs :		
18.1	No. of Vehicles used for collection of waste from member HCFs	:	(i) Four Wheelers:Nos and Vehicle Numbers: (ii) Two Wheelers :.....Nos and Vehicle Numbers:.....
18.2	Vehicles are labeled as per BMW Rules, 2016	:	☐ Satisfactory ☐ No satisfactory
18.3	Vehicles used are as per CPCB Guidelines	:	☐ Satisfactory ☐ No satisfactory

S.No.	Details		Particulars												
18.4	Vehicles attached with the GPS provision as per BMW Rules 2016		☐ Satisfactory ☐ No satisfactory												
18.5	Whether waste collected from member HCFs adopted Bar coding system ?		☐ Yes ☐ No												
19.0	Temporary untreated waste storage area	:	☐ Satisfactory ☐ No satisfactory												
20.0	Mode of conveyance of bio-medical waste from untreated waste storage area to the treatment equipment within the CBWTF	:	☐ Closed Trolley/Pull cart with bio-hazard symbol ☐ No Closed Trolley/Pull cart ☐ Others like												
21.0	Treatment equipment installed at CBWTF														
21.1	Incinerator/plasma pyrolysis capacity and make	:	(i) No. of Incinerators including standby: (ii) Incineration capacity: kg /hrKg/day.												
21.2	Daily Operation schedule of the incinerator /plasma pyrolysis (timings)	:	AM toPM (or)PM toAM Whether bio-medical waste collected from member HCFs is treated during holidays: Yes ☐ No ☐												
21.3	Consumption of auxiliary fuels	:	<table border="1"> <thead> <tr> <th>S. No</th><th>Type of Fuel</th><th>Consumption Quantity in liters per day</th><th>Bill numbers of purchase of fuel</th></tr> </thead> <tbody> <tr> <td>a)</td><td></td><td></td><td></td></tr> <tr> <td>b)</td><td></td><td></td><td></td></tr> </tbody> </table>	S. No	Type of Fuel	Consumption Quantity in liters per day	Bill numbers of purchase of fuel	a)				b)			
S. No	Type of Fuel	Consumption Quantity in liters per day	Bill numbers of purchase of fuel												
a)															
b)															
21.4	Stack attached with the incinerator /plasma pyrolysis	:	(i) Stack Diameter: m (ii) Stack Height : m above Ground Level												
21.5	Monitoring provision attached with the stack	:	☐ Platform ☐ Porthole ☐ access to the platform (Steps/Monkey Ladder/any other.....)												
21.6	Is stack monitoring provision satisfactory	:	☐ Yes ☐ No												

S.No.	Details		Particulars
	and as per CPCB guidelines		
21.7	air pollution control systems attached with the incinerator/plasma pyrolysis	:	(i) Quenching : ☐ Yes ☐ No (ii) Venturi scrubber : ☐ Yes ☐ No (iii) Droplet separator : ☐ Yes ☐ No (iv) Mist eliminator : ☐ Yes ☐ No (v) Filters : ☐ Yes ☐ No (vi) Lime and Activated Carbon injection: : ☐ Yes ☐ No (vii) ID Fan : ☐ Yes ☐ No (viii) Any other : (Pl. indicate)
21.8	Waste feeding mechanism	:	(i) Manual feeding : ☐ Yes ☐ No (ii) PLC based Automatic feeding : ☐ Yes ☐ No
21.9	Is PLC and automatic recording system (for recording operating parameters of the incinerator) attached with the incinerator/plasma pyrolysis	:	(i) PLC synchronized with waste feeding mechanism & in working condition: ☐ Yes ☐ No (l) PLC synchronized and recording system attached with incinerator and in working condition: ☐ Yes ☐ No
21.10	Operational conditions of the Incineration/plasma pyrolysis as observed during the visit	:	(i) Whether burners in working condition: ☐ Yes ☐ No (ii) Temperature maintained in Primary Chamber (range) :° C (iii) Temperature maintained in Secondary Chamber (range):.....° C (iv) Negative draft in Primacy Chamber :mm of water column (v) Pressure drop in the Venturi: mm of water column
21.11	Is continuous on-line monitoring system/Flue gas analyser attached with the incinerator/plasma pyrolysis for flue gas	:	(i) Is continuous online monitoring system (COMS) attached with incinerator: ☐ Yes ☐ No (ii) Observed values of flue gas parameters: CO ₂ : .%; O ₂ : % and CO: % (iii) Observed Combustion Efficiency:%

S.No.	Details		Particulars
	analysis (i.e CO, O ₂ and CO ₂)		(iv) Observed values of stack emissions as per COMS
21.12	Emergency and Fire safety measures adopted within the facility is adequate	:	Is Emergency stack attached with the incinerator: ☐ Yes ☐ No Whether fire safety measures adopted (Fire Extinguishers, Sand buckets etc.): ☐ Yes ☐ No
21.13	Log book for incinerator/ plasma pyrolysis is maintained and satisfactory	:	Log Book Maintained: ☐ Yes ☐ No Log Book Maintained is satisfactory : ☐ Yes ☐ No
21.14	Details of heat recovery system installed with incinerator/plasma pyrolysis	:	☐ Yes ☐ No
22.0	Capacity of autoclave and-- make	:	Autoclave of capacitykg/cycle and make installed.
22.1	Operating conditions of autoclave/microwave as observed during the visit	:	Operating parameters observed: (i) Temperature : in °C (ii) Pressure : in psi (iii) Residence time : in minutes
22.2	Provision made for the autoclave /microwave	:	Trolley for waste feeding : ☐ Yes ☐ No Graphic or computer recording device attached: ☐ Yes ☐ No
22.3	Spore test or strip test conducted regularly and records maintained	:	☐ Yes ☐ No Pl. indicate frequency of Strip test conducted: every batch /once in a week /quarterly /yearly Pl. indicate frequency of Spore test conducted: every batch /once in a week /quarterly /yearly
22.4	Performance of autoclave by spore testing or routine test	:	☐ Satisfactory ☐ Not satisfactory
22.5	Log book maintained for autoclave is satisfactory	:	Log Book Maintained: ☐ Yes ☐ No Log Book Maintained is satisfactory : ☐ Yes ☐ No
23.0	Capacity of shredder and make	:	 kg/hr. Self-designed & got fabricated locally.

S.No.	Details	Particulars														
24.0	Details of sharp pit / Encapsulation facility	(i) Sharp Pit provided : ☐ Yes ☐ No (ii) Is it as per CPCB guideline : ☐ Yes ☐ No (iii) Records maintained : ☐ Yes ☐ No (iv) Total quantity of waste sharps stored: (v) Total quantity of waste sharps treated and disposed:														
25.0	Water Balance															
25.1	Source and quantity of water intake per day (cu.m / day)	Water consumption source: Water is drawn at KLD approximately. Is magnetic water flow meter attached to the water source/water storage tank : ☐ Yes ☐ No Magnetic water flow meter readings as per record (for last month): 1 st Day of Month : Last day of month : Magnetic Flow meter as observed during the visit: <table border="1" style="margin-top: 10px;"> <thead> <tr> <th rowspan="2">S. No</th> <th rowspan="2">Month</th> <th colspan="2">Magnetic flow meter reading</th> </tr> <tr> <th>Initial</th> <th>Final</th> </tr> </thead> <tbody> <tr> <td>(1)</td> <td>Previous month</td> <td></td> <td></td> </tr> <tr> <td>(2)</td> <td>On the date of visit:.....</td> <td></td> <td></td> </tr> </tbody> </table> If water requirement is met from outside through tankers, pl. provide No. of Tankers procured in a previous six months: Total quantity of water consumed during the previous six months : in KLD	S. No	Month	Magnetic flow meter reading		Initial	Final	(1)	Previous month			(2)	On the date of visit:.....		
S. No	Month	Magnetic flow meter reading														
		Initial	Final													
(1)	Previous month															
(2)	On the date of visit:.....															
25.2	Break up of water usage (such as washing, scrubbing etc.)	Scrubber – KL/hr or KLD Washing – KLD Disinfections – KLD Gardening – KLD Domestic – KLD														

S.No.	Details		Particulars
26.0	Total wastewater effluent generated per day	:	AboutKLD generated Quantity of treated water reused/recycled in %: Any other mode of disposal:
27.	Effluent treatment plant details		
27.1	ETP Capacity	:	 KL/Cycle
27.2	Flow Chart of ETP	:	ETP comprising of: Unit operations
27.3	Intake and Discharge of ETP	:	(i) Magnetic Flow measuring device provided at the outlet of ETP: ☐ Yes ☐ No (ii) Energy meter attached to the ETP: ☐ Yes ☐ No (iii) Energy consumed over a period of one month: = Units (iv) pH meter attached at the outlet of ETP: ☐ Yes ☐ No
27.4	Final mode of disposal of treated water	:	(i) Is treated wastewater complying with the discharge norms ☐ Yes ☐ No (ii) Is Treated water is reused in the scrubber: ☐ Yes ☐ No (ii) Is Treated water is reused for gardening: ☐ Yes ☐ No (iii) Is Treated water is discharged in drain: ☐ Yes ☐ No (iv) Is Treated water is discharged in open area: ☐ Yes ☐ No
28.	Status of infrastructure provided (Pl. indicate 'Yes / No' whichever is applicable)		
28.1	Separate treatment equipment room	:	☐ Yes ☐ No
28.2	Main waste storage room	:	☐ Yes ☐ No
28.3	Treated waste storage room	:	☐ Yes ☐ No
28.4	Administrative room	:	☐ Yes ☐ No
28.5	Generator set	:	☐ Yes ☐ No

S.No.	Details		Particulars
	(i) Capacity	:	
	(ii) Is Stack attached as per DG Set norms	:	☐ Yes ☐ No
	(iii) Is Acoustic enclosure provided as per DG Set norms	:	☐ Yes ☐ No
	(iv) Is DG Set complying to the emissions norms and noise level norms	:	☐ Yes ☐ No If so, pl. indicate latest monitoring results:
28.6	Site security (high walls, fencing, guarded gates etc.)	:	High walls on all four sides : ☐ Yes ☐ No Fencing on all the sides : ☐ Yes ☐ No Guarded Gates : ☐ Yes ☐ No Any other observation pl indicate:.....
28.7	Parking facility	:	☐ Yes ☐ No
28.8	Sign board	:	☐ Yes ☐ No
28.9	Green belt	:	☐ Yes ☐ No
28.10	Washing room	:	☐ Yes ☐ No
28.11	First aid box	:	☐ Yes ☐ No
28.12	Lighting arrangements in the facility	:	☐ Yes ☐ No
28.13	Odour problem remedial measures	:	☐ Yes ☐ No
28.14	Fire fighting and emergency facilities	:	☐ Yes ☐ No
28.15	Measures for control of pests / insects etc.	:	☐ Yes ☐ No
28.16	Protective gear for waste handlers	:	☐ Yes ☐ No
28.17	Telephone facility	:	☐ Yes ☐ No
28.18	Provision of washing, toilets and safe place for eating for the workers	:	☐ Yes ☐ No
28.19	Fire alarm system provided in the facility	:	☐ Yes ☐ No

S.No.	Details		Particulars
29.	Record maintenance and record keeping details (Pl. indicate 'Yes / No' whichever is applicable)		
29.1	Waste Movement /Manifest record	:	☐ Yes ☐ No
29.2	Log book for treatment equipment	:	☐ Yes ☐ No
29.3	Site records	:	☐ Yes ☐ No
29.4	Incineration ash generation and final disposal records	:	☐ Yes ☐ No
29.5	Treated plastic waste generation and its sale to the registered recycler	:	☐ Yes ☐ No
29.6	Syringes treated and its final disposal record	:	☐ Yes ☐ No
29.7	Workers health status records		☐ Yes ☐ No
29.8	Workers immunization records		☐ Yes ☐ No
29.9	Medical and para-medical workers training records		☐ Yes ☐ No
29.10	Whether records maintained with regard to the accidents (such as fire, spills and injury and measures taken)		☐ Yes ☐ No
30.	Collection and transportation status (Yes / No)*		
30.1	Whether waste collected in a container of similar colour with label as per the Rules?	:	☐ Yes ☐ No
30.2	Whether the person who collects BMW maintain a register with him / her?	:	☐ Yes ☐ No

S.No.	Details		Particulars
30.3	Has due attention have been given in vehicles to prevent spillage / pilferage/ loading / unloading etc.?	:	☐ Yes ☐ No
30.4	Is the vehicle labeled with the symbol and display the name, address, telephone number etc.?	:	☐ Yes ☐ No
30.5	Does the CBWTF operator use satellite station to store the waste?	:	☐ Yes ☐ No (If yes, give details.....)
30.6	The CBWTF operator collects waste daily or alternate day including holidays?	:	☐ Yes ☐ No
30.7	Whether waste treatment criterion of 48 hours is complied?		☐ Yes ☐ No
31.	Disposal of treated waste:		
31.1	Plastic waste after treatment	:	Plastic waste Sold to: M/s. and approved bySPCB/PCC
31.2	Treated sharps	:	Treated syringes disposal by:..... or through M/s.....and approved bySPCB/PCC
31.3	Incineration ash	:	Incineration ash disposal by: Disposal in Sanitary Landfill: ☐ Yes ☐ No Disposal through TSDF: ☐ Yes ☐ No Any other mode :.....
31.4	Other treated solid wastes	:	
31.5	Oil & grease	:	
31.6	Treated wastewater	:	


S.No.	Details		Particulars																					
32.	Frequency of incinerator / autoclave / microwave / hydroclave / ETP discharge effluent testing and name of the laboratory (specify approved or not under E(P) Act, 1986 or NABL Accredited Lab.). Give details of compliance / non-compliance)	:	(i) Reported monitoring frequency: (ii) Stack monitoring : Quarterly : ☐ Yes ☐ No (iii) Waste water : Monthly/Quarterly/Yearly (iv) Incineration ash : Monthly/Quarterly/Yearly (v) Name of the Laboratory conducted test: (vi) Is the Laboratory approved under E (P) Act, 1986/.....SPCB/PCC/ NABL: : ☐ Yes ☐ No (vii) Copies of the analysis reports of treated effluent, incinerated ash, stack monitoring as (Annexures.....)																					
32.1	Frequency of site inspection by SPCBs/PCCs/CPCB/any other agencies	:	(i) No. of times in a year inspected by the SPCB/PCC: (ii) No. of times in a year inspected by the CPCB																					
33.	Monitoring Results :																							
33.1	Incinerator stack emission (parameters stipulated in the Rules, temperature attainment in the chambers, residence time in the secondary chamber etc.)	:	<table border="1"> <thead> <tr> <th>Parameter</th><th>PM</th><th>HCl</th><th>NOx</th><th>Hg & com-pounds</th><th>Dioxins and Furans</th><th>C.E.</th></tr> </thead> <tbody> <tr> <td>Date</td><td></td><td></td><td></td><td></td><td></td><td></td></tr> <tr> <td>LIMIT</td><td>50</td><td>50</td><td>400</td><td>0.05</td><td>0.1 ng TEQ per Nm³</td><td>99.00%</td></tr> </tbody> </table> Date of monitoring: Note: All values are in mg/Nm ³ , except CE	Parameter	PM	HCl	NOx	Hg & com-pounds	Dioxins and Furans	C.E.	Date							LIMIT	50	50	400	0.05	0.1 ng TEQ per Nm ³	99.00%
Parameter	PM	HCl	NOx	Hg & com-pounds	Dioxins and Furans	C.E.																		
Date																								
LIMIT	50	50	400	0.05	0.1 ng TEQ per Nm ³	99.00%																		
33.2	Whether Stack emission norms are complied with by the CBWTF		☐ Yes ☐ No																					
33.3	Incineration ash characteristics	:	Characteristics as per Schedule –II of HOW (M& TM) Rules,2016 (Annexure-----) Is it hazardous waste as per HOWM&TM Rules, 2016: ☐ Yes ☐ No																					
33.4	ETP inlet/outlet characteristics	:	<table border="1"> <thead> <tr> <th>Parameter</th><th>pH</th><th>TSS</th><th>COD</th><th>BOD</th><th>O&G</th></tr> </thead> <tbody> <tr> <td>ETP Inlet Result</td><td></td><td></td><td></td><td></td><td></td></tr> </tbody> </table>	Parameter	pH	TSS	COD	BOD	O&G	ETP Inlet Result														
Parameter	pH	TSS	COD	BOD	O&G																			
ETP Inlet Result																								

S.No.	Details		Particulars					
			ETP Result	Outlet				
			All values are in mg/l except pH					
33.5	Whether liquid effluent discharge norms are complying by the CBWTF	:	☐ Yes ☐ No					
33.6	Whether CBWTF is submitting the annual report within the due date for the preceding year	:	☐ Yes ☐ No If Yes, annual report submitted vide letter No..... dated.....					
34.	Any other relevant observations	:	(pl. enclose as annexure)					
35.	Name of the officials with designation inspected /monitored the CBWTF and the signature	:						

Annexure-VI

STATIONARY SOURCE EMISSION MONITORING

MODIFICATIONS TO BE MADE TO SAMPLING PLATFORM AND SAMPLING PORT HOLE

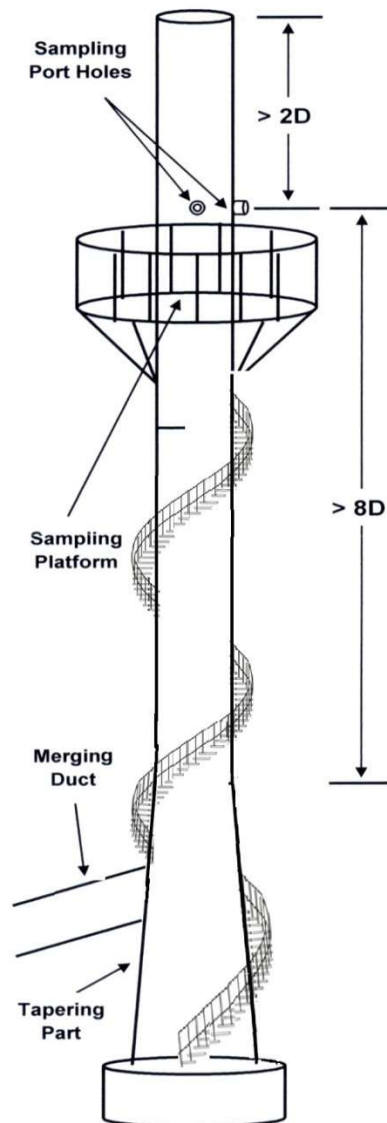


Number of Port Holes : Minimum two numbers of Port Holes at 90° apart from each other at a horizontal plane.

Location of Port Holes : Minimum 8 times of Internal Diameters of Stack downstream (upward direction of stack) from any duct confluence, bends and tapering & minimum 2 times of Internal Diameters of Stack upstream (downward direction of stack) from stack exit.


Location of Sampling Platform : 5 feet upstream (downward direction of stack) from the Port Hole as determined above.

Port Hole Flange : If the internal diameter of the flange is 4 inch or more then there is no need to change, if it is less than 4 inch then it has to be replaced with 4 inch flange. The flange should not protrude out more than 6 inches from the outer wall of the stack (it shall be kept as less as possible).


Sampling Platform Modification : A semi-circular extension of the existing platform (width extending outward by 6 feet from outside wall of the stack and covering at least one third of the circumference) may be provided for access to both the Port Holes. This area can be extended from the existing Platform and if deemed necessary for safety of the personnel a counter extension in opposite direction may also be provided. The extended Platform shall be strengthened with requisite support from the stack.

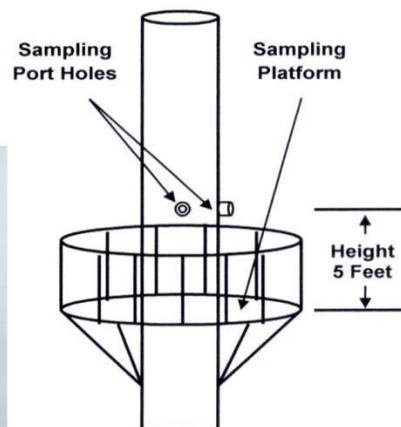


Note: Alternatively, safe access to monitoring platform may be provided with separate scaffolding-cum-staircase arrangement

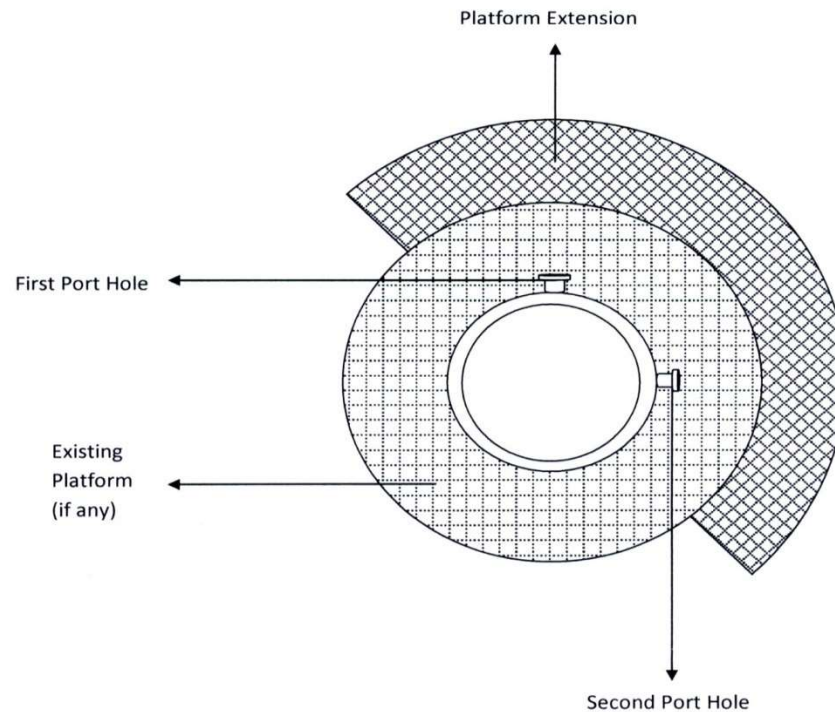

Sampling Platform Modification / Extension

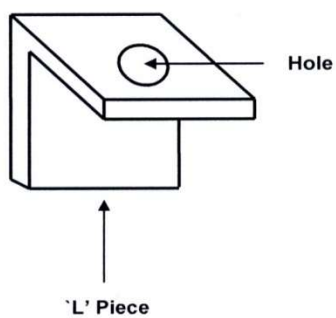

Fixing of 'L' Pieces on the stack wall : Two 'L' shaped pieces are to be fixed on the stack wall for mounting the Mono-Rail & Chain (part of the Sampling Kit for movement of sampling Train in & out through the Sampling Port Hole). The 'L' pieces shall be made of approximately 6 mm thick galvanized iron to have 5 cm long arms. One arm of the 'L' piece shall be welded on the stack wall and another arm shall have a hole of 14 mm diameter near the open end. Both the 'L' Pieces shall be welded on the stack wall at specified distances (as shown in the diagram on the next page) from the centre of Sampling Port Hole (in a vertical axis on the Stack Wall).

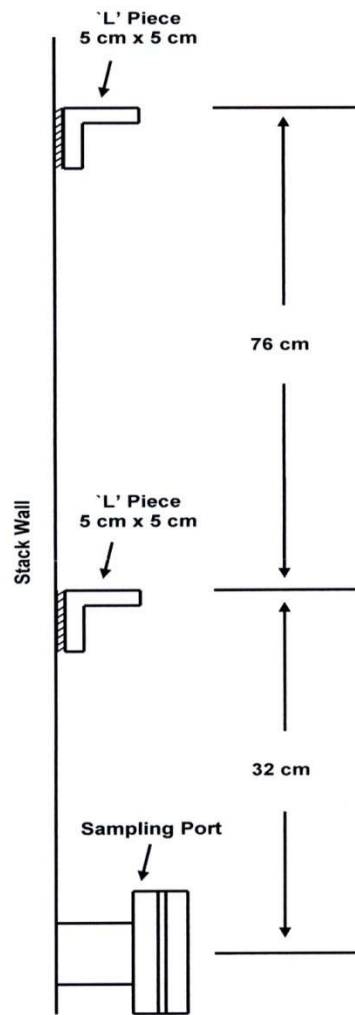

Fixing of 'L' Pieces on the Stack Wall

ANNEXURE – VII

The vehicle shall be labeled with the bio-hazard symbol (as per Schedule IV of the BMWWM Rules) and should display the name, address and contact telephone and mobile number of the CBWTF.

Bio Medical Waste Vehicle

Name and address of CBWTF with Contact number of CBWTF operator

Authorized by (Name of) State Pollution Control Board/Pollution Control Committee

Vehicle Side-1**Bio Medical Waste Vehicle**

Name and address of CBWTF with Contact number of CBWTF operator

Authorized by (Name of) State Pollution Control Board/Pollution Control Committee

Vehicle Side-2



Bio- Hazard symbol at back side of the vehicle

Note: Proportion of Font size with respect to body height of the vehicle-12:1 (Minimum)

Proportion of Bio-hazard symbol with respect to body height of the vehicle-12:3 (Minimum)

Example: If body height is 6 feet i.e. 72" then minimum font size will 6" and minimum size of bio-hazard symbol will be 18".

REFERENCES

1. Bio-medical Waste Management Rules, 2016.
2. Revised Guidelines for Common Bio-medical Waste Treatment Facilities (2016).
3. CPCB Guidelines for BMW Incinerators.
4. 'Disposal of Bio-medical Waste generated during Universal Immunization Programme' issued by CPCB.
5. 'Guidelines for Environmentally Sound Management of Mercury Waste Generated from the Health Care Facilities' issued by CPCB.
6. Annual Report 2023 submitted to CPCB by the SPCBs/PCCs.
7. Stationary Source Emission Monitoring –Modifications to be made to the Sampling Platform and Sampling Port Hole issued by National Reference Trace Organics Laboratory (NRTOL), CPCB.

-- OO --

- TRUE COPY -

By Speed Post

F. No. B-31011-BMW (3398)-2023-WM-I

October 10, 2023

To,

The Member Secretary,
All SPCB and PCC

Sub: Regarding methodology to conduct gap analysis with respect to generation and treatment of biomedical waste -reg.

Sir/Madam,

It is to inform that State Pollution Control Boards/Pollution Control Committees are required to conduct gap analysis with respect to generation and treatment of biomedical waste in respective State/UT. A format for conducting gap analysis is given in CPCB guidelines for Common Bio-medical Waste Treatment Facilities. Few State Boards have prepared gap analysis report adopting their own methodology. The matter was also discussed in Central Monitoring Committee meeting on 18.07.2023 wherein need for adopting uniform methodology was emphasised. Hence, to avoid the ambiguity and to adopt uniform procedure, CPCB has prepared a methodology to conduct gap analysis (Copy attached herewith for ready reference).

In view of above, it is requested to kindly conduct gap analysis with respect to generation and treatment of biomedical waste in your State/UT using the aforesaid methodology and report may be submitted to CPCB within one month.

Yours faithfully,



(V. P. Yadav)

Director & Head

Waste Management -I Division

Encl. As above

Copy to:

i. PS to 'MS'

: For kind information of 'MS' please



(V. P. Yadav)

केन्द्रीय प्रदूषण नियंत्रण बोर्ड

निर्गत

दिनांक

18/10/2023

0/c

Methodology to Conduct gap analysis with respect to generation and treatment of biomedical waste

Guidelines for Common Biomedical Waste Treatment Facilities was prepared by CPCB with an aim to have uniformity in ensuring site selection, allowing and establishment of a state-of-the-art Common Biomedical Waste Treatment Facilities (CBWTFs), operation as well as verification of compliance to the BMWM Rules, 2016 throughout the country. As per the said guideline, SPCB/PCC is required to prepare an inventory or review with regard to the bio-medical waste generation at least once in five years in the coverage areas of the existing CBWTF and conduct gap analysis as per format given in Annexure-I of the guideline.

To avoid the ambiguity and maintaining the uniformity for conducting gap analysis a methodology is suggested for estimating generation, treatment of biomedical waste and its extrapolation in the State and coverage area of CBMWTF. It is elaborated in following table.

S. No.	Parameters	Details
1.	Coverage area of CBWTF	Up to 75 km
2.	No. of HCFs (Bedded and non-bedded)	In Number
3.	No. of Beds covered	In Number
4.	Total biomedical waste generation (in Kg/day)	The generation may be calculated considering following factors: a) Generation from Bedded hospital (in absence of availability of required information biomedical waste generation may be taken as 274 grams per bed) b) Biomedical waste generated from non-bedded HCFs and other sources also be considered
5.	Extrapolate the biomedical waste generation for next years	Extrapolation may be based on factors such as population growth of the districts/cities covered by CBWTF, Rate of increase in number of HCFs/beds in past years etc. as decided by SPCB in consultation with Health department and CBMWTF associations.
6.	Total existing treatment capacity (in Kg/day) (Sum of Incineration Capacity and Autoclave/Microwave/Hydroclave Capacity)	For calculation of existing treatment capacity, maintenance time may be considered for calculating operational hours of equipment as below: a) Operational Hours for static incinerator 20 hrs/day b) Operational hours for Rotary incinerator 22 hrs/day

		c) 18 cycle per day for autoclave The actual capacity may be considered as 90% of available capacity keeping 10% margin for diverted/extra waste etc.
7.	Total Biomedical Waste treated and disposed (Kg/day)	Sum of all categories of biomedical waste treated and disposal.
8.	Gap between total extrapolated biomedical waste generation (for next 10 years) and existing biomedical waste treatment capacity	Extrapolate the biomedical waste generation minus total existing treatment capacity

Based on the above data, the gap between existing treatment capacity and need of additional treatment capacity should be examined after carrying out gap analysis at coverage area/city level and State level.



Service - Reply of R5 - MPCC in matter - Amresh Singh Vs State of UP & Ors. - OA 1141/2024

From Mansi Bachani <mansi@eldfindia.com>
Date Tue 12/16/2025 12:39 PM
To mreshsingh0085@gmail.com <amreshsingh0085@gmail.com>; daleepdhayani@yahoo.co.in <daleepdhayani@yahoo.co.in>; priyanka swami <advpriyankaswami@gmail.com>; anujbhandari123@gmail.com <anujbhandari123@gmail.com>
Cc su@chambersofsanjayupadhyay.com <su@chambersofsanjayupadhyay.com>; Surya Gupta <surya@eldfindia.com>; anubhavanand200201@gmail.com <anubhavanand200201@gmail.com>; eldflegal@gmail.com <eldflegal@gmail.com>; admin <admin@chambersofsanjayupadhyay.com>

 1 attachment (12 MB)
16.12.2025 - SU_ for filingAffidavit in compliance of order dt 20.11.2025 - Amresh Singh (1) (2)_pagenumber.pdf;

Dear Ma'am/Sir,

Please Find Attached the Reply on behalf of R5 - MPCC in compliance of 20.11.2025 in the matter titled Amresh Singh Vs State of UP & Ors. - OA 1141/2024.

Thanks and Regards,
Mansi Bachani
Advocate and Partner
Enviro Legal Defence Firm
Mobile: +91-8600531203
Email: mansi@eldfindia.com
Web:www.eldfindia.com

New Delhi Office: 29, Presidential Estate; LGF; Nizamuddin (East) New Delhi-110013; Ph No. +91-11-40573181

NOTE: *Law Firms in India are not allowed to have websites as per Bar Council Rules. If you want to know more about Enviro Legal Defence Firm contact the address above. Incidentally, ELDF is India's first environmental law firm!*